



Standard Test Method for Determination of Trace Thiophene in Refined Benzene by Gas Chromatography¹

This standard is issued under the fixed designation D 4735; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This test method covers the determination of thiophene in refined benzene in the range from 0.5 mg/kg to 5.0 mg/kg. The range of the test method may be extended by modifying the sample injection volume, calibration range, or sample dilution with thiophene-free solvent.

1.2 This test method has been found applicable to benzene characteristic of the type described in Specifications D 2359 and D 4734 and may be applicable to other types or grades of benzene only after the user has demonstrated that the procedure can completely resolve thiophene from the other organic contaminants contained in the sample.

1.3 The following applies to all specified limits in this test method: for purposes of determining conformance with this test method, an observed value or a calculated value shall be rounded off "to the nearest unit" in the last right-hand digit used in expressing the specification limit in accordance with the rounding-off method of Practice E 29.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.* For specific hazard statements, see Section 7.

2. Referenced Documents

2.1 ASTM Standards:

- D 1193 Specification for Reagent Water²
- D 1685 Test Method for Traces of Thiophene in Benzene by Spectrophotometry³
- D 2359 Specification for Refined Benzene-535³
- D 3437 Practice for Sampling and Handling Liquid Cyclic Products³
- D 4734 Specification for Refined Benzene 545³
- E 29 Practice for Using Significant Digits in Test Data to Determine Conformance with Specifications⁴

¹ This test method is under the jurisdiction of ASTM Committee D-16 on Aromatic Hydrocarbons and Related Chemicals and is the direct responsibility of Subcommittee D16.0E on Instrumental Analysis.

Current edition approved Feb. 10, 1996. Published April 1996. Originally published as D 4735 – 87. Last previous edition D 4735 – 87 (1991) ^{ϵ 1}.

² *Annual Book of ASTM Standards*, Vol 11.01.

³ *Annual Book of ASTM Standards*, Vol 06.04.

⁴ *Annual Book of ASTM Standards*, Vol 14.02.

E 260 Practice for Packed Column Gas Chromatography⁴
E 840 Practice for Using Flame Photometric Detectors in Gas Chromatography⁴

2.2 Other Document:

OSHA Regulations, 29 CFR, paragraphs 1910.1000 and 1910.1200⁵

3. Summary of Test Method

3.1 The thiophene concentration in refined benzene is determined at the milligram thiophene per kilogram sample level using conventional gas-liquid chromatography with a flame photometric detector. A reproducible volume of sample is injected. Quantitative results are obtained by the external standard technique using the measured peak area of thiophene.

4. Significance and Use

4.1 This test method is suitable for setting specifications on benzene and for use as an internal quality control tool where benzene is either produced or used in a manufacturing process.

4.2 This test method was found applicable for determining thiophene in refined benzene conforming to the specifications described in Specification D 2359 and may be applicable toward other grades of benzene if the user has taken the necessary precautions as described in the text.

4.3 This test method was developed as an alternative technique to Test Method D 1685.

5. Apparatus

5.1 *Gas Chromatograph*—Any chromatograph having a flame photometric detector may be used which can operate at the typical conditions described in Table 1. The user is referred to Practice E 260 for additional information about gas chromatography principles and procedures.

5.2 *Column*—The column must provide complete resolution of thiophene from benzene and any other hydrocarbon impurities because of potential quenching effects by hydrocarbons on the light emissions from the thiophene. The columns described in Table 1 have been judged satisfactory.

5.3 *Detector*—Any flame photometric detector (FPD) can be used, provided it has sufficient sensitivity to produce a minimum peak height twice that of the base noise for a 4- μ L

⁵ Available from Superintendent of Documents, U.S. Government Printing Office, Washington, DC 20402.

TABLE 1 Thiophene in Benzene Instrumental Conditions

	A	B	C
Column			
Tubing	6 ft × 1/8 in. Ni Steel	15 ft by 1/8 in. stainless steel	10 ft by 1/8 in. stainless steel
Phase	TCEPE ^A	SP-1000	OV-351
Concentration, weight %	7	10	10
Support	Chromosorb P-AW ^B	Supelcoport	Chromosorb P-AW
Mesh	100/120	60/80	80/100
Detector			
H ₂ , mL/min	140	140	140
Air I, mL/min	80	80	80
Air II, mL/min	170	170	170
Gas chromatographic conditions			
Inlet, °C	150	170	180
Detector, °C	220	220	250
Carrier Gas	helium	helium	helium
Flow Rate, mL/min	30	30	30
Column Temperature, °C	70	90	70

^A Tetracyanoethylated pentaerythritol or pentrite.

^B Chromosorb P is a registered trademark of the Manville Corp.

injection volume of 0.5 mg/kg thiophene in benzene. The user is referred to Practice E 840 for assistance in optimizing the operation and performance of the FPD.

5.4 *Integrator*—Electronic integration is recommended.

5.5 *Recorder*, a-c, 1-mV range strip chart recorder is recommended.

5.6 *Microsyringe*, 10- μ L capacity.

5.7 *Volumetric Flasks*, 50, 100 and 500-mL capacity.

5.8 *Separatory Funnel*, 1-L capacity.

6. Reagents and Materials

6.1 *Purity of Reagents*—Reagent grade chemicals shall be used in all tests. Unless otherwise indicated, it is intended that all reagents shall conform to the specifications of the Committee on Analytical Reagents of the American Chemical Society, where such specifications are available.⁶ Other grades may be used, provided it is first ascertained that the reagent is of sufficiently high purity to permit its use without lessening the accuracy of the determination.

6.2 *Purity of Water*—Unless otherwise indicated, reference to water shall be understood to mean reagent water conforming to Type IV of Specification D 1193.

6.3 *Carrier Gas*, nitrogen or helium, chromatographic grade.

6.4 *Hydrogen*, zero grade.

6.5 *Compressed Air*, hydrocarbon-free.

6.6 *Cadmium Chloride Solution* (20 g/L)—Dissolve 20 g of anhydrous cadmium chloride CdCl₂ into 200 mL of water and dilute to 1 L.

6.7 *Isatin Solution*⁷—Add 0.5 g of isatin to 200 mL of chloroform. Heat under a fume hood to a temperature just below the boiling point of chloroform (61°C) and maintain for

5 min with stirring. Filter the hot solution through hardened rapid-filter paper into a 250-mL volumetric flask and dilute to volume.

6.8 *Benzene, Thiophene-Free*—Wash 700 mL of benzene in a 1000-mL separatory funnel to which has been added 5 mL of isatin solution, with successive 100-mL portions of concentrated sulfuric acid until the H₂SO₄ layer is light yellow or colorless. Wash the benzene with 100 mL of water, then twice with 100 mL of cadmium chloride solution (CdCl₂). Finally, wash with another 100-mL portion of water and filter the benzene through medium filter paper into a storage bottle, stopper the bottle tightly and save for future use.

6.9 *Sulfuric Acid*—Concentrated H₂SO₄.

6.10 *Thiophene*⁸.

7. Hazards

7.1 Benzene is considered a hazardous material. Consult current OSHA regulations and supplier's Material Safety Data Sheets, and local regulations for all materials used in this method.

8. Sampling and Handling

8.1 Sampling of benzene should follow safe rules in order to adhere to all safety precautions as outlined in the latest OSHA regulations. Refer to Practice D 3437 for proper sampling and handling of benzene.

9. Preparation of the Apparatus

9.1 The chromatographic separation of trace level sulfur compounds can be complicated by absorption of the sulfur compounds by the gas chromatographic system. Therefore, care should be taken to properly free the system of active sites where absorption or reactions could take place.

9.2 Follow the manufacturer's instructions for mounting the column into the gas chromatograph and adjusting the instrument to conditions described in Table 1. Allow the instrument and detector sufficient time to reach equilibrium.

⁶ *Reagent Chemicals, American Chemical Society Specifications*, American Chemical Society, Washington, DC. For suggestions on the testing of reagents not listed by the American Chemical Society, see *Analar Standards for Laboratory Chemicals*, BDH Ltd., Poole, Dorset, U.K., and the *United States Pharmacopeia and National Formulary*, U.S. Pharmaceutical Convention, Inc. (USPC), Rockville, MD.

⁷ Isatin 2,3-indolinedione such as Aldrich Catalog No. 11,461-8, available from Aldrich Chemical Co., Inc., 940 W. Saint Paul Ave., Milwaukee, WI 53233, or equivalent has been found satisfactory for this purpose.

⁸ Thiophene such as Aldrich Catalog No. T3,180-1, available from Aldrich Chemical Co., Inc., 940 W. Saint Paul Ave., Milwaukee, WI 53233, or equivalent has been found satisfactory for this purpose.

10. Calibration Curve

10.1 Prepare a 500-mL stock solution of thiophene in benzene at the 100 mg/kg level by adding 0.04 g (38.0 μL) of thiophene to 435 g (500 mL) of thiophene-free benzene.

10.2 Calculate the thiophene content of the stock solution according to the following equation:

$$\text{Thiophene, mg/kg} = (A \times 10^3)/B$$

where:

A = weight of thiophene, mg, and

B = weight of benzene, g.

10.3 Prepare five calibration blends ranging from 0.00 to 10.0 mg/kg of thiophene in benzene by diluting the appropriate volume of stock solution into a known volume of thiophene-free benzene.

10.4 For example, an 87.0 mg/kg stock solution was prepared by dissolving 0.0378 g thiophene into 435 g of benzene. Aliquots of 0.00, 0.75, 1.0, 2.0, and 5.0 mL of stock solution were dissolved in 100 mL of thiophene-free benzene to produce 0.00, 0.65, 0.87, 1.75, and 4.35 mg/kg, respectively.

10.5 Inject 4.0 μL of each solution into the chromatograph. Integrate the area under the thiophene peak. Each standard solution and the blank should be analyzed in triplicate.

NOTE 1—Injection volumes must be consistent and reproducible.

10.6 Prepare a calibration curve by plotting the integrated peak area versus milligram per kilogram of thiophene on a sheet of log/log graph paper.

NOTE 2—In the sulfur mode, the FPD will exhibit a response that is a nonlinear power law function. Please refer to Practice E 840 for additional information on the characteristics and usage of the FPD.

11. Procedure

11.1 Charge 4.0 μL of sample into the chromatograph.

11.2 Measure the area of the thiophene peak. The measurement of the sample peak should be consistent with the method for measuring peak areas in the calibration blends. A typical chromatogram is shown in Fig. 1 representing 1.10 mg/kg thiophene in benzene.

12. Calculation

12.1 Determine the amount of thiophene directly from the calibration curve prepared in 10.6.

13. Report

13.1 Report the thiophene concentration to the nearest 0.01 mg/kg.

14. Precision and Bias

14.1 *Precision:*

14.1.1 The following criteria should be used to judge the acceptability of the 95 % probability level of the results obtained by this test method. The criteria were derived from a round robin between five laboratories. The data were obtained over 2 days using different operators.

14.1.2 *Intermediate Precision (formerly called Repeatability)*—Results in the same laboratory should not be considered suspect unless they differ by more than the amount shown in Table 2.

14.1.3 *Reproducibility*—The results submitted by two laboratories should not be considered suspect unless they differ by more than the amount shown in Table 2.

14.2 *Bias*—The bias in this test method is being determined.

15. Keywords

15.1 benzene; flame photometric detector; gas chromatography; thiophene

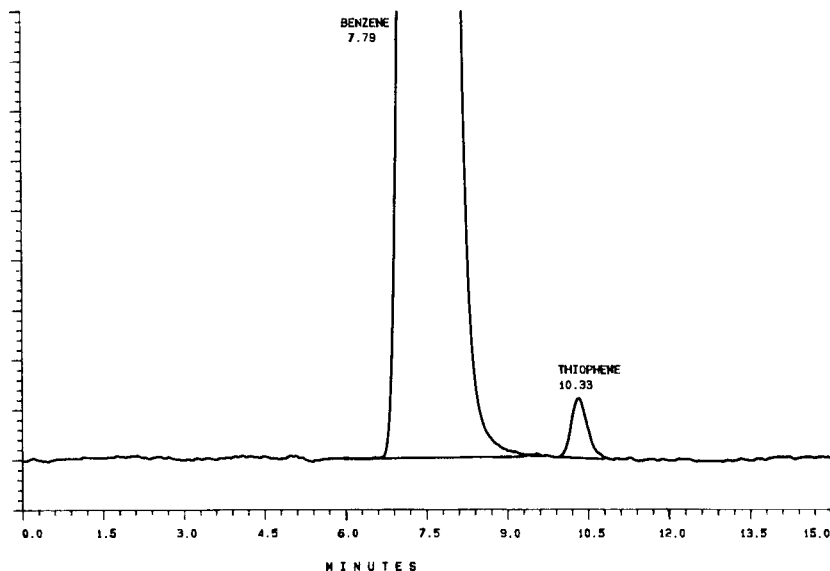


FIG. 1 Chromatogram Illustrating the Analysis of 1.10 mg/kg Thiophene in Benzene

TABLE 2 Intermediate Precision and Reproducibility

Thiophene Concentration, mg/kg	Repeatability, mg/kg	Reproducibility, mg/kg
0.80	0.040	0.060
1.80	0.078	0.078

The American Society for Testing and Materials takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, 100 Barr Harbor Drive, West Conshohocken, PA 19428.