



# Standard Test Method for Measuring the Electromagnetic Shielding Effectiveness of Planar Materials<sup>1</sup>

This standard is issued under the fixed designation D 4935; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope

1.1 This test method provides a procedure for measuring the electromagnetic (EM) shielding effectiveness (SE) of a planar material due to a plane-wave, far-field EM wave. From the measured data, near-field SE values may be calculated for magnetic (H) sources for electrically thin specimens.<sup>2,3</sup> Electric (E) field SE values may also be calculated from this same far-field data, but their validity and applicability have not been established.

1.2 The measurement method is valid over a frequency range of 30 MHz to 1.5 GHz. These limits are not exact, but are based on decreasing displacement current due to decreased capacitive coupling at lower frequencies and on overmoding (excitation of modes other than the transverse electromagnetic mode (TEM)) at higher frequencies for the size of specimen holder described in this test method. Any number of discrete frequencies may be selected within this range. For electrically thin, isotropic materials with frequency-independent electrical properties of conductivity, permittivity and permeability, measurements may be needed at only a few frequencies as the far-field SE values will be independent of frequency. If the material is not electrically thin or if any of the parameters vary with frequency, measurements should be made at many frequencies within the band of interest.

1.3 This test method is not applicable to cables or connectors.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee D-9 on Electrical and Electronic Insulating Materials and is the direct responsibility of Subcommittee D09.12 on Electrical Tests.

Current edition approved April 10, 1999. Published June 1999. Originally published as D 4935-89. Last previous edition D 4935-89 (1994) <sup>$\epsilon$ 1</sup>.

<sup>2</sup> Wilson, P. F., and Ma, M. T., "A Study of Techniques for Measuring the Electromagnetic Shielding Effectiveness of Materials," NBS Technical Note 1095, May 1986.

<sup>3</sup> Adams, J. W., and Vanzura, E. J., "Shielding Effectiveness Measurements of Plastics," NBSIR 85-3035, January 1986.

## 2. Referenced Documents

2.1 *ASTM Standards:*

D 1711 Terminology Relating to Electrical Insulation<sup>4</sup>

## 3. Terminology

3.1 *Definitions*—For definitions of terms used in this test method refer to Terminology D 1711.

3.2 *Definitions of Terms Specific to This Standard:*

3.2.1 *dynamic range (DR)*—the difference between the maximum and minimum signals measurable by the system.

3.2.1.1 *Discussion*—Measurement of materials with good SE require extra care in order to avoid contamination of extremely low power or voltage values by unwanted signals from leakage paths.

3.2.2 *electrically thin*—the thickness of the specimen is much, much ( $<1/100$ ) less than the electrical wavelength within the specimen.

3.2.3 *far field*—that region where E and H are orthogonal to each other and also to the direction of propagation of energy.

3.2.4 *near field*—that region where E and H are not related by simple rules.

3.2.4.1 *Discussion*—The transition region between near field and far field is not abrupt, but occurs approximately  $\lambda/2\pi$  from a dipole source, where  $\lambda$  is the free-space wave length of the frequency of the source. This concept of regions is further blurred by reradiating due to scattering by reflecting materials or objects that may be distant from the source. The interior of metallic structures often contains a mixture of near-field regions.

3.2.5 *shielding effectiveness (SE)*—the ratio of power received with and without a material present for the same incident power.

3.2.5.1 *Discussion*—It is usually expressed in decibels by the following equation:

$$SE = 10 \log \frac{P_1}{P_2} \text{ (decibels, dB)} \quad (1)$$

where:

<sup>4</sup> *Annual Book of ASTM Standards*, Vol 10.01.

$P_1$  = received power with the material present, and  
 $P_2$  = received power without the material present.

If the receiver readout is in units of voltage, use the following equation:

$$SE = 20 \log \frac{V_1}{V_2} \text{ (decibels, dB)} \quad (2)$$

where:

$V_1$  and  $V_2$  are the respective voltage levels with and without a material present.

According to these equations, SE will have a negative value if less power is received with the material present than when it is absent.

#### 4. Significance and Use

4.1 This test method applies to the measurement of SE of planar materials under normal incidence, far-field, plane-wave conditions (E and H tangential to the surface of the material).

4.2 The uncertainty of the measured SE values is a function of material, mismatches throughout the transmission line path, dynamic range of the measurement system, and the accuracy of the ancillary equipment. An uncertainty analysis is given in Appendix X1 to illustrate the uncertainty that may be achieved by an experienced operator using good equipment. Deviations from the procedure in this test method will increase this uncertainty.

4.3 Approximate near-field values of SE may be calculated for both E or H sources by using measured values of far-field SE. A program may be generated from the source code in Appendix X2 that is suitable for use on a personal computer.

4.4 This test method measures the net SE caused by reflection and absorption. Separate measurement of reflected and absorbed power may be accomplished by the addition of a calibrated bidirectional coupler to the input of the holder.

#### 5. Apparatus

5.1 A basic equipment setup is shown in Fig. 1.

5.2 *Specimen Holder*—Physical dimensions of a specimen holder are given in the annex. The specimen holder is an enlarged, coaxial transmission line with special taper sections and notched matching grooves to maintain a characteristic impedance of 50  $\Omega$  throughout the entire length of the holder. This impedance is checked in accordance with 7.1, and any variations greater than  $\pm 0.5 \Omega$  are corrected. There are three important aspects to this design. First, a pair of flanges in the middle of the structure hold the specimen. This allows capacitive coupling of energy into insulating materials through displacement current. Second, a reference specimen of the same thickness and electrical properties as the load specimen causes the same discontinuity in the transmission line as is caused by the load specimen. Third, non-conductive (nylon) screws are used to connect the two sections of the holder together during tests. This prevents conduction currents from dominating the desired displacement currents necessary for the correct operation of this specimen holder.




FIG. 1 General Test Setup

5.3 *Signal Generator*—A source capable of generating a sinusoidal signal over the desired portion of the frequency range specified in 1.2. A 50- $\Omega$  output impedance is needed to minimize reflections due to mismatches. Precision step attenuators are useful in increasing the effective dynamic range for SE measurements.

5.4 *Receiver*—A device with a 50- $\Omega$  input impedance capable of measuring signals over the same frequency range as the signal generator in 5.3. A wide dynamic range is desirable in order to achieve a wide dynamic range of measured SE values. Typically, either a spectrum analyzer or a field intensity meter is used.


5.5 *Coaxial Cables and Connectors*—These are devices for connecting power between specific components without causing interference with other components. These should all have a 50- $\Omega$  characteristic impedance. Double-shielded cables provide lower leakage than single-shielded cables. Type-N connectors provide more reliability and less leakage than BNC connectors. Precision 14-mm connectors give lower mismatch errors and are more reliable under heavy usage than other connectors, but are more expensive and are not used on most generators or receivers.

5.6 *Attenuators*—These are devices used to isolate the specimen holder from the signal generator and the receiver. Their main purpose in this system is for impedance matching. A 10-dB, 50- $\Omega$  attenuator should be used on each end of the specimen holder. The material under test usually causes a large reflection of energy back into the signal generator. This may also cause variations of the incident power by changing the generator impedance loading. Use of a bidirectional coupler allows monitoring and correcting any changes in incident power due to this loading. Attenuators greater than 10 dB will excessively decrease the dynamic range of the measurement system.

#### 6. Test Specimens

6.1 The reference and load specimens must be of the same material and thickness. Both are shown in Fig. 2. Dimensions are shown in Fig. 3. The load specimen can be larger than the outer diameter of the flange on the holder, but keeping them to the dimensions shown in Fig. 3 will expedite handling.

6.2 Specimen thickness is a critical dimension. For the best repeatability of SE measurements, reference specimen and load specimen must be identical in thickness. For this method, two

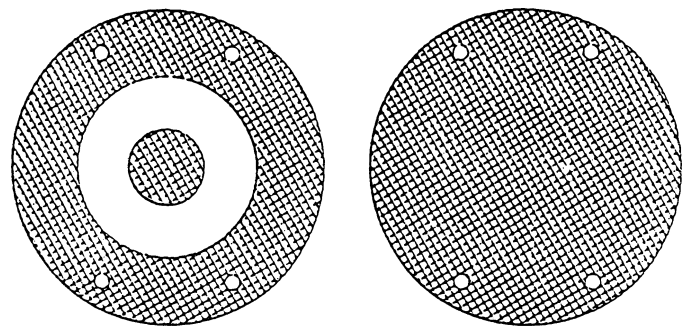

REFERENCE

LOAD

FIG. 2 Illustration of Reference and Load Specimens

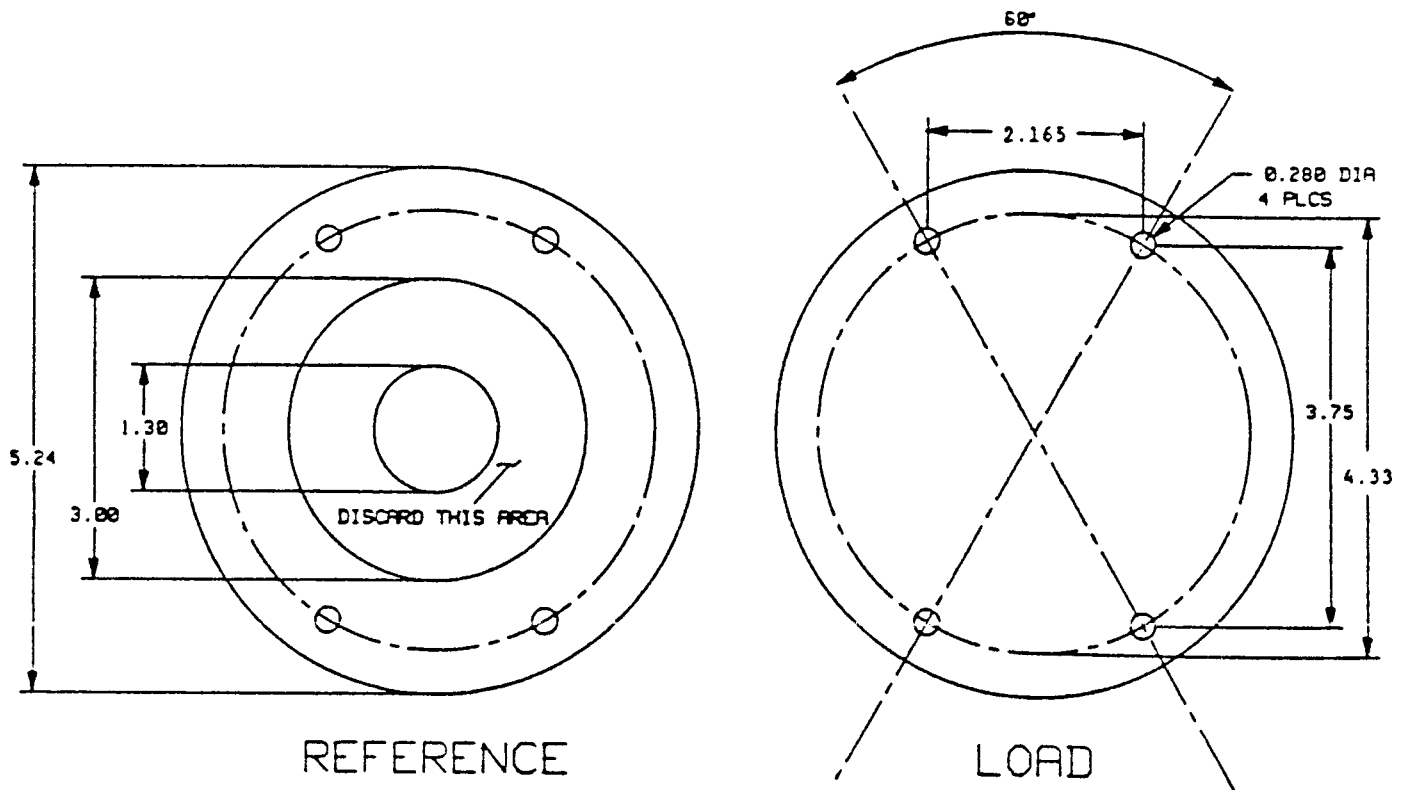


FIG. 3 Drawing That Gives Dimensions of Reference and Load Specimens

specimens are considered to have identical thickness if the difference in the average thicknesses is less than 25  $\mu\text{m}$  and the thickness variation within and between specimens is less than 5 % of the average.

6.3 Materials of the specimens may be either homogeneous or inhomogeneous, single or multiple layered, and conducting or insulating. Measured SE values of inhomogeneous materials are dependent on geometry and orientation, and results are less repeatable than for homogeneous materials.

6.4 Before tests, condition test specimens for 48 h at  $23 \pm 2^\circ\text{C}$  and  $50 \pm 5\%$  relative humidity. Tests must be performed immediately upon removal from conditioning environment.

### 7. Preparation of Apparatus

7.1 An initial check of the specimen holder should be performed with a time-domain reflectometer or other suitable instrument in order to ensure that a characteristic impedance of  $50 \pm 0.5 \Omega$  has been achieved during construction, and that this impedance has not been degraded during shipment or handling. A time-domain system can give location of a mismatch in addition to its magnitude.

7.2 Each time the ancillary equipment is connected to the specimen holder, good practice requires measurement of a reference specimen in order to ensure the measurement system is in proper working order.

7.2.1 The dynamic range of the system can be checked by comparing the maximum signal level obtained with a reference specimen to the minimum signal level obtained when using a metallic load specimen. The lower limit of the measurement system sensitivity is a function of the sensitivity and bandwidth

of the receiver. Narrowing the bandwidth of the receiver lowers the detectable level, but increases the measurement time. Leakage due to connectors or cables may reduce the DR of the system by providing a parallel signal path that does not pass through the specimen. If a step attenuator placed in series with the specimen holder causes a change in the minimum signal detected that corresponds to a change in attenuator setting, and if the step attenuator itself does not cause a leakage path, leakage is negligible and the DR measured above is correct. If the levels do not correspond, the attenuation should be increased until a one-to-one correspondence is achieved to determine the DR. Since leakage from a coaxial connector is determined not only by the quality of the connector, but also by the amount of torque used in tightening the connector, connections should be rechecked.

7.2.2 If a standard reference specimen such as gold film deposited on mylar is available, measurement of its value can provide assurance that the entire system is working properly. A specimen that has 5  $\Omega$  per square resistance should give a measured SE of  $-32 \pm 3 \text{ dB}$ . Any other known specimen may be used to check setup-to-setup repeatability.

7.2.3 Careful handling of the specimen holder and specimens is important.

7.3 Preparation of 7.2 should be run in accordance with procedures of Section 8.

### 8. Procedure

8.1 Follow the preparation of apparatus in accordance with 7.2 whenever the measurement system has been reconfigured or not used for several days.

8.2 Prepare two specimens in accordance with Section 6.

8.3 Determine all frequencies for which SE values are to be measured. The specimen mounting procedure described in 8.4 requires more time and effort than changing frequency, so it is more efficient to record values at all frequencies for the reference specimen, change to the load specimen, and then record load values at these same frequencies. This procedure can be automated if a computer and ancillary equipment with IEEE-488 Bus capability are available.

8.4 The procedure for inserting the specimens is as follows: Use a support structure (a large roll of tape or special stand) to support the specimen holder in a vertical position. Remove two nylon screws, turn the holder end for end, remove the other two nylon screws, and carefully lift off the upper half of the holder. An indented, soft foam pad is useful for holding this upper half of the specimen holder while continuing the installation or removal of specimens. Place the two pieces of the reference specimen on the flange of the bottom half of the specimen holder, taking care that the disk for the center conductor is aligned correctly. Use small amounts of transparent tape as needed. Replace the half of the specimen holder that had been removed so that the holes for the nylon screws are aligned. Reinstall two nylon screws. Turn the holder end for end and then reinstall the other two nylon screws. Reconnect the coaxial cables.

8.5 Measure the received power (or voltage) while using the reference specimen. Record the measured received values as  $P_2$  or  $V_2$  values at each frequency.

8.6 Replace the reference specimen with the load specimen.

8.7 Measure the received power with the load specimen. Record these measured values as  $P_1$  or  $V_1$  values at the same frequencies used in 8.5. If this value is within 10 dB of the smallest detectable signal of the measurement system, either the receiver bandwidth must be decreased and the measurement repeated, or the SE value is beyond the dynamic range of the measurement system and hence the SE value is reported as exceeding the DR of the system.

8.8 If the recorded units were watts, use the power ratio equation (1) to calculate SE. If the recorded units were volts, use the voltage ratio Eq 2 from 3.2.5 to calculate SE.

## 9. Report

9.1 The report should give test specimen identification and measured values of SE at each frequency of measurement.

9.2 Values of SE based on measured values from 8.7 that were within 10 dB of the smallest detectable signal of the measurement system should be noted as exceeding the DR of the measurement system.

## 10. Precision and Bias

10.1 Precision and bias are inherently affected by the choice of apparatus and specimens. For analysis and details, see Appendix X1.

## 11. Keywords

11.1 electromagnetic shielding; far field; near field; shielding; shielding effectiveness (SE)

## ANNEX

### (Mandatory Information)

#### A1.


A1.1 This annex contains a set of figures suitable for use in the construction of a specimen holder which has been shown to produce reliable measurements. They were contributed by the National Institute of Standards and Technology (formerly NBS). Corrections to these figures were contributed by W. E. Measurements.<sup>5</sup>

A1.2 These figures are for one half of two identical halves of the specimen holder.

A1.2.1 Additional parts required are Type N male connectors (two required) and ¼ by 20 by 1 nylon screws (four required). The Type N connector is Midwest Microwave number 2679M.<sup>6</sup>

<sup>5</sup> A complete specimen holder is available from W. E. Measurements, P.O. Box 18056, Boulder, CO 80308.

<sup>6</sup> Available from Midwest Microwave Inc., 3800 Packard Road, Ann Arbor, MI 48104.

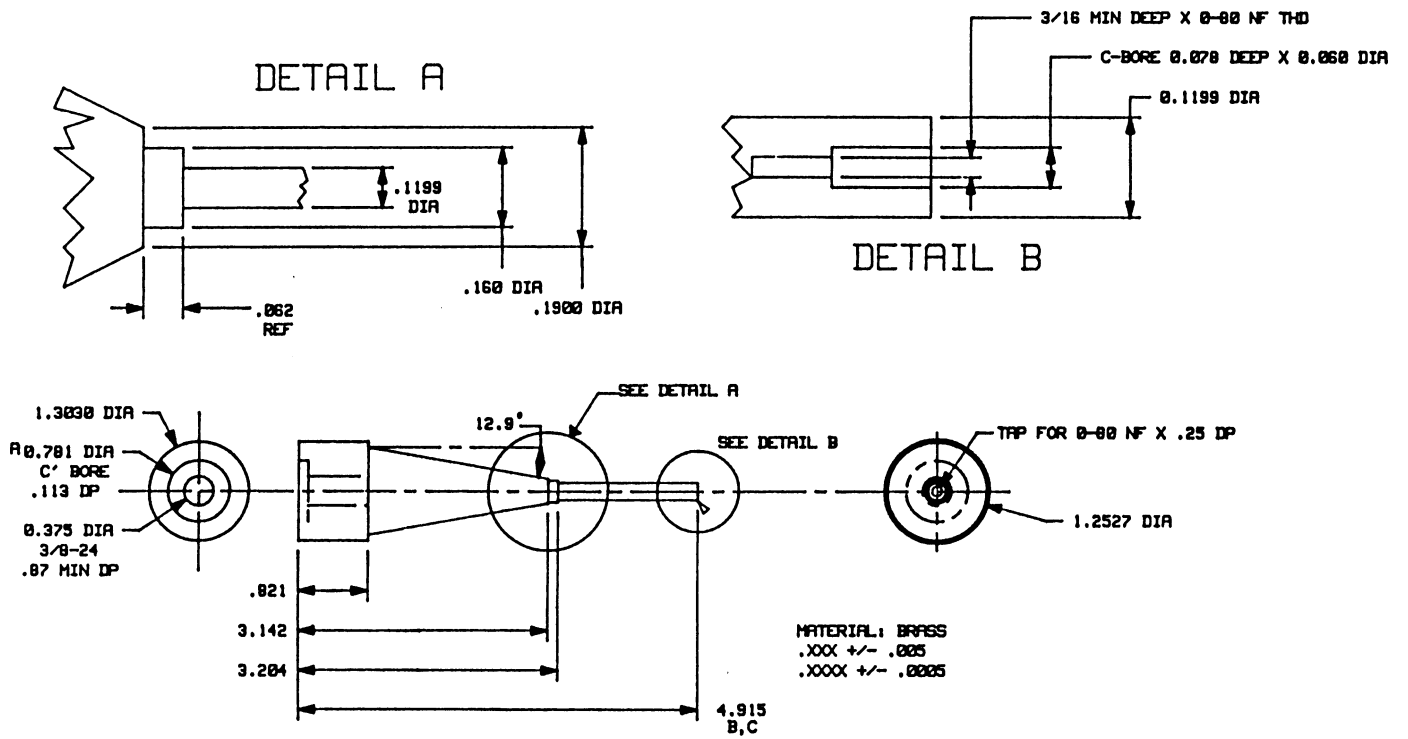

NOTES:

- A. PRESS FIT WITH PART C.
- B. MAKE +.050 ASSEMBLE AND ADJUST
- C. TO BE ASSEMBLED AND LENGTH CUT TO SAME LENGTH AS PART G, .3743 ± LENGTH

PART A

FIG. A1.1 Part A, Taper Section for Center Conductor

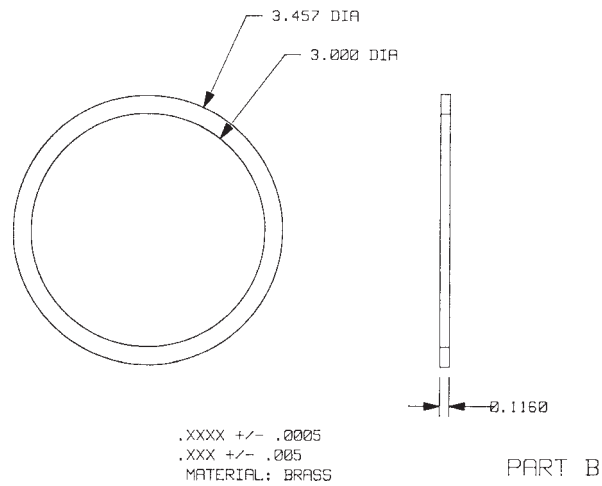
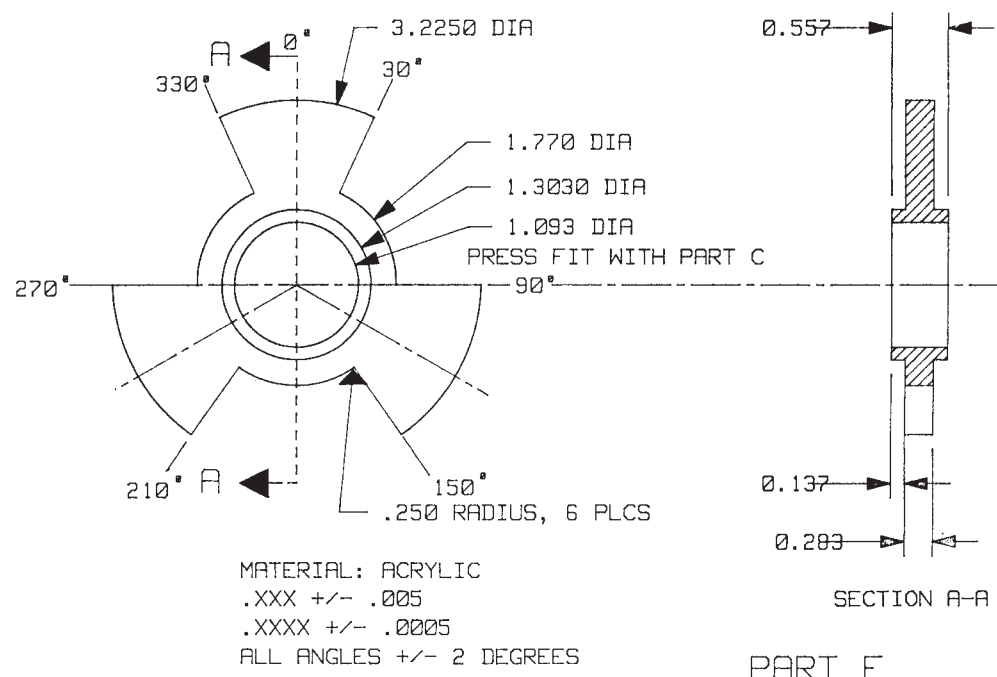
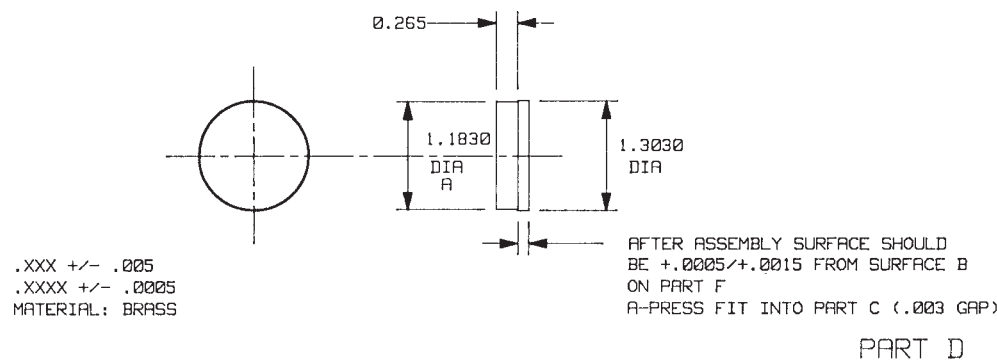
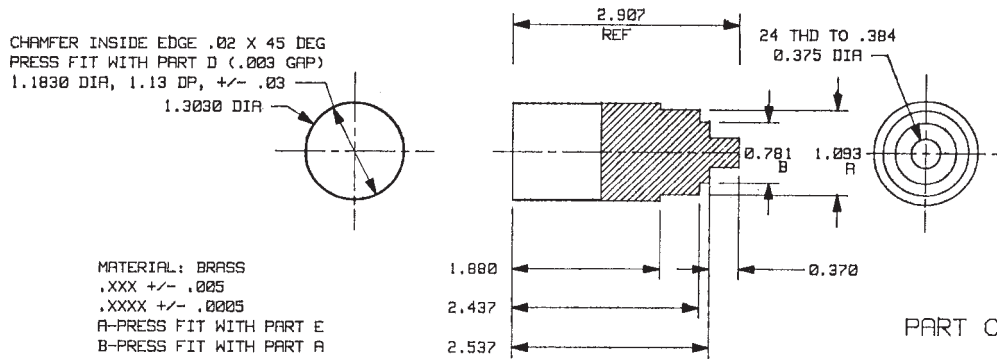


FIG. A1.2 Part B, Pressure Ring for Outer Conductor



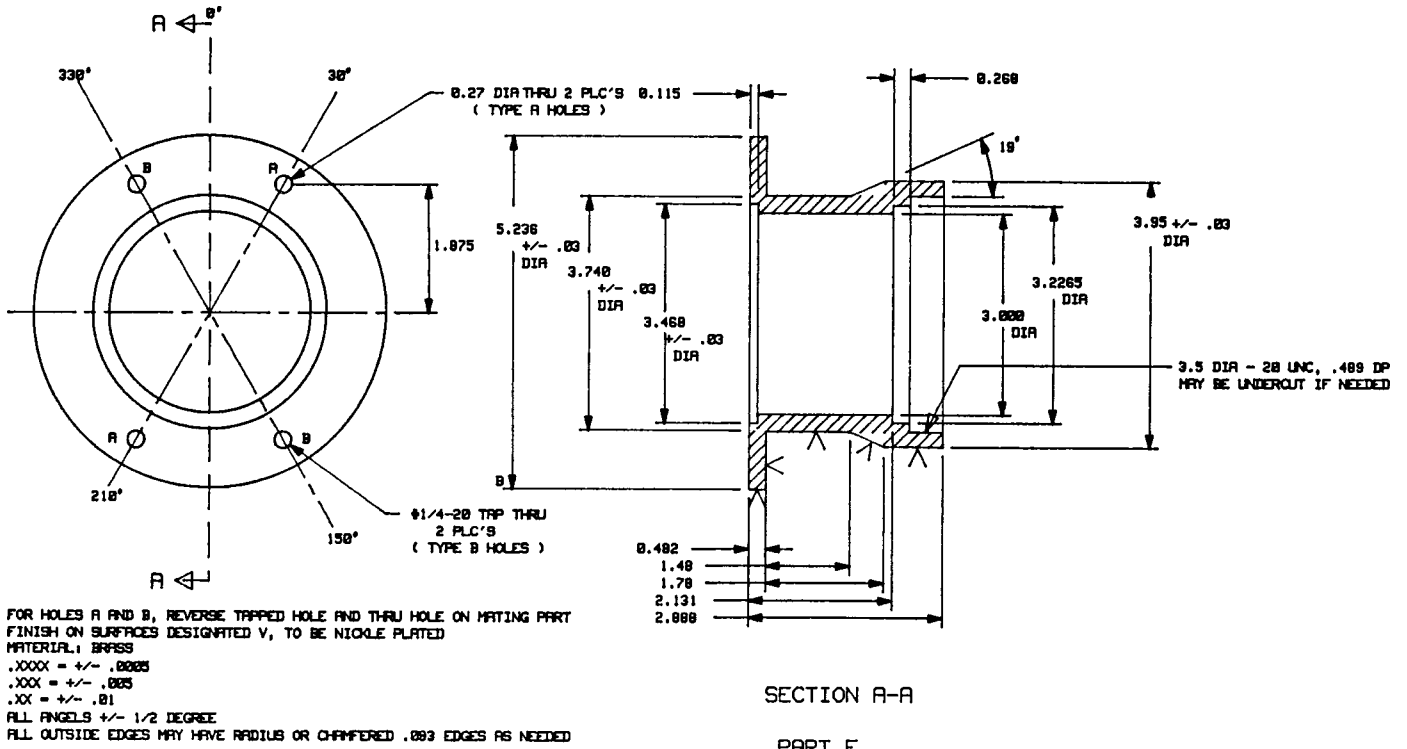


FIG. A1.6 Part F, Flange Section of Outer Conductor



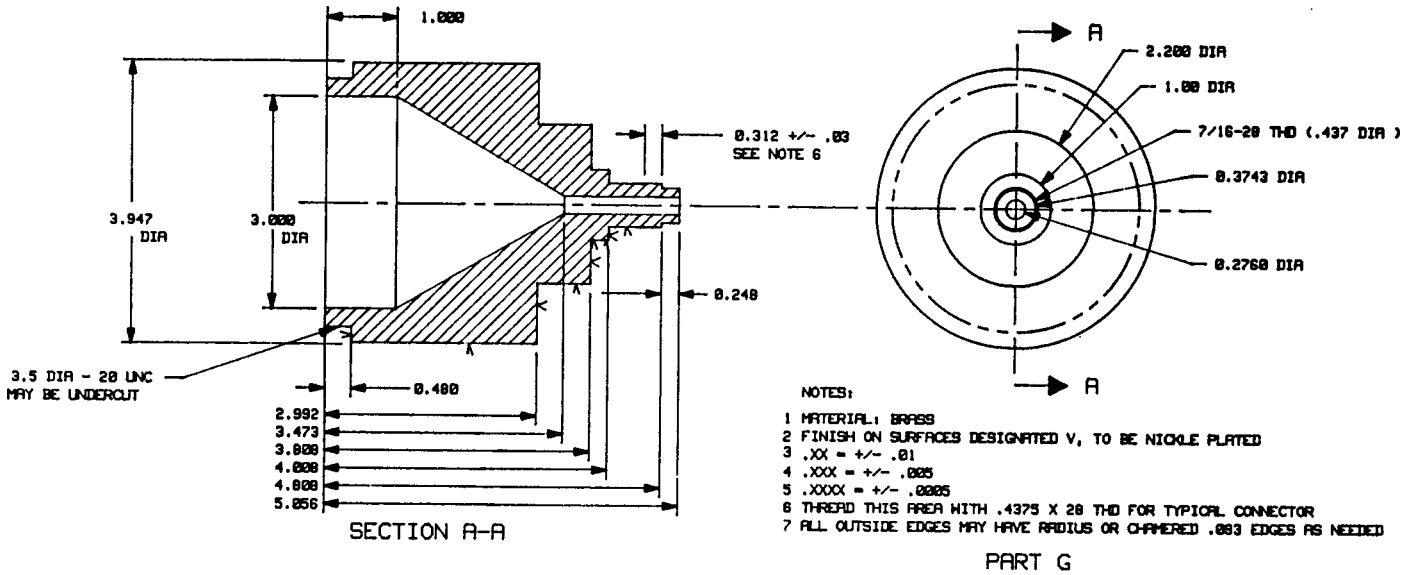


FIG. A1.7 Part G, Taper Section for Outer Conductor

## SAMPLE HOLDER ASSEMBLY



**FIG. A1.8 Assembly Drawing for a Half Section**

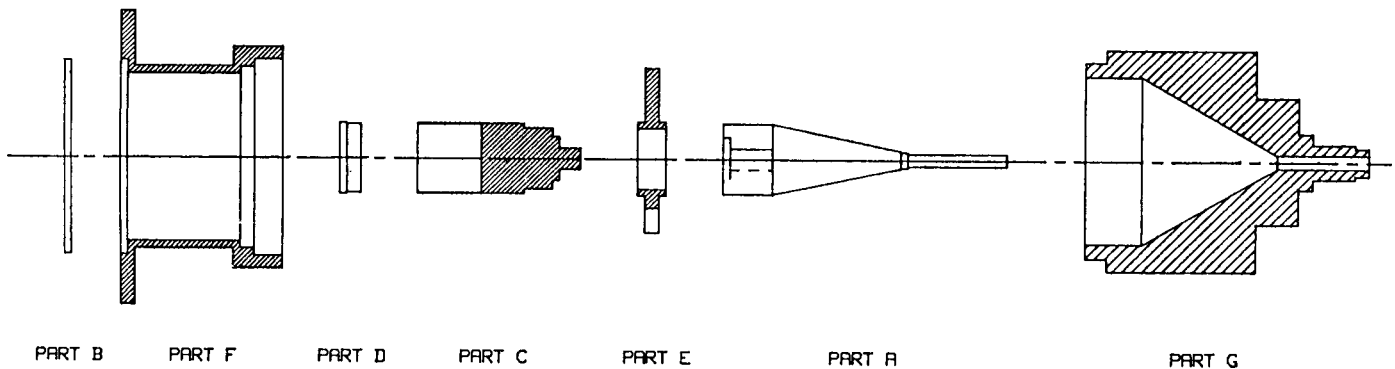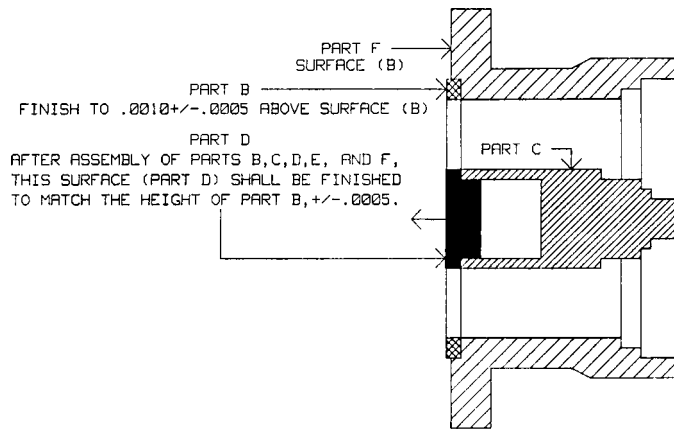

PARTIAL ASSEMBLY SHOWING FLANGE MACHINING DETAILS

**FIG. A1.9 Partial Assembly Drawing**

## APPENDIXES

### (Nonmandatory Information)

#### X1. ESTIMATE OF UNCERTAINTY OF SE MEASURED VALUES

X1.1 This appendix gives an estimate of uncertainty in the measured values of SE. The sources of error considered are operator errors, specimen-caused errors, and measurement-system errors.

X1.2 Operator errors may be caused by either carelessness or lack of experience and training. No bound can be placed on such errors, but the deviation from any norm may be large enough that an experienced observer will be able to determine that the results are indeed erroneous.

X1.3 Specimen-caused errors are due to irregularities in specimens, either in preparation or in inherent structure. Isotropic, homogeneous specimens with smooth surfaces will give the most repeatable results. If the reference specimen and load specimen are of different thickness, a bias error will be introduced. If both specimens are of the same thickness, but

have irregular thickness over each specimen, random errors will be introduced. Inhomogeneities or anisotropies in specimens cause various effects depending on size, distribution, and geometric arrangement. Experience with measurements on many types of specimens indicates that repeatability of measured data may be expected except when the surface is rough. A round-robin of measurements made on different types of specimens bears this out.

X1.4 Measurement-system errors are caused by impedance mismatches, generator instabilities, leakage paths, limited dynamic range, limited frequency range and receiver errors. To the extent that an experienced, well-trained operator can make measurements over the appropriate frequency range, within the dynamic range of the system, avoid leakage paths within the measurement system's dynamic range, use suitable attenuators

to avoid mismatches, monitor and adjust input power to keep it constant, then measurement-system errors may be reduced to a very modest part of the total error.

X1.5 Table X1.1 gives a summary of estimated errors under favorable conditions by a skilled operator.

X1.6 The systematic error in the receiver is probably irrelevant since the SE values are based on difference measurements. The random error that relates to drift over a few minute time period is very relevant. If no attenuators were used, the mismatch error on the generator side would be excessive, since, in one case, with the reference specimen installed in the holder, the impedance seen by the signal generator is determined almost entirely by the receiver, and, in the other case, with the load specimen installed, the impedance seen by the signal generator is almost a short circuit for conductive specimens. The actual change in impedance is greatly reduced by the attenuator between the signal generator and the specimen holder. The actual change of impedance level seen by the signal generator may also load the signal generator and cause the output power to vary from one condition to the other. These changes can be monitored by use of a bi-directional coupler, and corrections can be made to compensate for them. This

**TABLE X1.1 Summary of Estimated Incertainties**

Source	Systematic	Random
Mismatch	±0.5 dB	±0.5 dB
Power instability in signal generator	±0.4 dB	±0.4 dB
Receiver calibration	±0.3 dB	±0.1 dB
Total	±1.2 dB	±1.0 dB

## X2. COMPUTER PROGRAM FOR CALCULATING NEAR-FIELD SE VALUES

X2.1 This appendix contains a short computer program for use with a personal computer. The program calculates near-field values of (SE) based on measured values of far-field SE. It produces approximate values, and as explained in Footnote 2, these values vary as a function of many factors, and therefore they should be used as estimates only. There are several approximations that apply. Nevertheless, these calculated values may serve as guidelines by providing knowledge concerning approximate near-field SE values without having to make the much more difficult measurements necessary to obtain either the near-field electric (E) or magnetic (H) SE values.

X2.2 The source file is written in (ASCII) code for an appropriate Fortran-77 compiler. Executable versions that do not require compilation are available for computers with or without math coprocessors.

X2.3 Three inputs are required, the positive measured SE value in dB of a material that has a flat frequency response from 100 to 1000 MHz, the separation distance between 2 coaxially oriented magnetic dipoles, and the separation distance between 2 coaxially oriented electric dipoles.

coupler is not shown as part of the setup shown in Fig. 1, so the error given for generator instability is based on no compensation. The size of the corrections measured with a coupler were the basis to determine the magnitude of this effect if no compensation is used.

X1.7 Results from a round robin of measurements performed by 5 different individuals at 5 different organizations on 5 sets of specimens of 3 different materials indicate what level of agreement may be expected. These results reflect variations due to all causes. Results from all 5 sets are not included, since a few data points are obvious outliers, probably caused by operator error. One material, stainless steel deposited on an ABS base, had a very smooth surface. The standard deviation for this specimen based on measurements by 5 individuals on 5 specimens was 0.9 dB. A second material, carbon coated on 1 side of an ABS base, was not quite as smooth, and the standard deviation for this specimen based on measurements by 5 individuals on 5 specimens was 2.0 dB. The third material, nickel coated on an ABS base, showed substantial surface roughness. The standard deviation for this specimen based on measurements by 5 individuals on 5 specimens was 6.0 dB. For all three materials, the same specimen holder and numbered specimens were used. Each of the 5 individuals used different ancillary equipment.

X1.8 The systematic uncertainty, or bias error, is ±1.2 dB. The random error, based on a standard deviation of 2.5 dB from the round robin results on reasonably smooth specimens, is within ±5 dB.

X2.4 The approximations made in the computer program are that  $k_0 * Z_0 \ll 1$ , that the material is electrically thin, and that  $Z_0 - D \approx Z_0$

where:

$Z_0$  = separation distance between the elemental dipoles, and

$D$  = specimen thickness. If the measured SE curve is not flat with frequency or if the material is anisotropic or multilayered, these approximations are not valid.

X2.5 Frequencies between 1 and 1000 MHz are used; values for SE for near-field E and near-field H are calculated. The output is in tabular form. The first column is frequency in MHz, the second column is SE of near-field H, the third column is SE of near-field E, and the fourth column repeats the input values of far-field SE. All SE values are in dB. The data may be directed into an ASCII file by use of the Disk Operating System (DOS) pipe command '>filename' for conversion to input data for spreadsheet and graphing programs.

X2.6 The computer program is shown in Fig. X2.1.

```

C
C
PROGRAM SE
C
THIS PROGRAM SHOULD BE VALID AS LONG AS KO*ZO << 1, THE MATERIAL
C IS ELECTRICALLY THIN, AND ZO=D-ZO. THIS TYPICALLY WILL RESTRICT
C THE UPPER FREQUENCY LIMIT TO AROUND 1 GHZ.
C
REAL PI,NO,KO,IL,ZO,W0
COMPLEX J,STH
PI=4.*ATAN(1.)
J=(0.,1.)
C=3.E+08
EO=(1.E-09)/36./PI
NO=120.*PI
FR=1.E+06
PRINT *, 'Insertion Loss in dB>0 ? '
READ (*,*) IL
C
Try ZO= 0.035 as a default value for Mag dipole separation.
C
PRINT *, 'Separation distance (m) between Magnetic dipoles?'
READ (*,*) ZO
C
Try EO= 0.090 as a default separation for E field dipoles.
C
PRINT *, 'Separation distance (m) between Electric dipoles?'
READ (*,*) W0
SD=2.*(10**(IL/ZO.)-1.)/NO
DO 30 I=1,3
DO 20 II=1,10
IF (II.EQ.1.AND.I.GT.1) GO TO 20
FREQ=II*FR
W=2.*PI*FREQ
KO=W/C
STH=J*KO*ZO*NO*SD/6.
ASEH=20.*ALOG10(CABS(1.+STH))
STE=NO*SD/KO/W0
ASEE=20*ALOG10(STE)
FF=20.*ALOG10(1.+5*NO*SD)
FM=FREQ/(1.0E+06)
PRINT 10,FM,ASEH,ASEE,FF
10 FORMAT(1X,4(1X,F8.2)/)
20 CONTINUE
FR=10.*FR
30 CONTINUE
END

```

**FIG. X2.1 ASCII Source Code for Fortran Compiler to Generate Program for Calculating Near-field SE Values From Measured Far-field SE Values**

*The American Society for Testing and Materials takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.*

*This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.*

*This standard is copyrighted by ASTM, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org).*