



Designation: D 1385 – 88 (Reapproved 2001)

## Standard Test Method for Hydrazine in Water<sup>1</sup>

This standard is issued under the fixed designation D 1385; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

### 1. Scope

1.1 This test method covers<sup>2</sup> the colorimetric determination of hydrazine in boiler feed waters, condensates, natural, and well waters that have been treated with hydrazine ( $N_2H_4$ ). This test method is usable in the range from 5.0 to 200  $\mu\text{g/L}$  (ppb) hydrazine. The range is for photometric measurements made at 458 nm in 50 mm cell. Higher concentrations of hydrazine can also be determined by taking a more diluted sample.

1.2 It is the users' responsibility to ensure the validity of this test method for untested types of waters.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.* For specific precautionary statements, see 5.3, Note 1, and Footnote 8.

### 2. Referenced Documents

#### 2.1 ASTM Standards:

- D 1066 Practice for Sampling Steam<sup>3</sup>
- D 1129 Terminology Relating to Water<sup>3</sup>
- D 1192 Specification for Equipment for Sampling Water and Steam in Closed Conduits<sup>3</sup>
- D 1193 Specification for Reagent Water<sup>3</sup>
- D 3370 Practices for Sampling Water from Closed Conduits<sup>3</sup>
- E 60 Practice for Photometric and Spectrophotometric Methods for Chemical Analysis of Metals<sup>4</sup>
- E 275 Practice for Describing and Measuring Performance of Ultraviolet, Visible, and Near Infrared Spectrophotometers<sup>5</sup>

### 3. Terminology

#### 3.1 Definitions—For definitions of terms used in this test

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee D19 on Water and is the direct responsibility of Subcommittee D19.03 on Sampling of Water and Water-Formed Deposits, Surveillance of Water, and Flow Measurement of Water.

Current edition approved March 28, 1988. Published May 1988. Originally published as D 1385 – 67. Last previous edition D 1385 – 86.

<sup>2</sup> For further information on this test method, the following references may be of interest: Watt, G. W., and Chrisp, J. D., "Spectrophotometric Method for the Determination of Hydrazine," *Analytical Chemistry*, Vol 24, No. 12, 1952, pp. 2006–2008, and Wood, P. R., "Determination of Maleic Hydrazide Residues in Plant and Animal Tissue," *Analytical Chemistry*, Vol 25, No. 12, 1953, pp. 1879–1883.

<sup>3</sup> *Annual Book of ASTM Standards*, Vol 11.01.

<sup>4</sup> *Annual Book of ASTM Standards*, Vol 03.05.

<sup>5</sup> *Annual Book of ASTM Standards*, Vol 03.06.

method, refer to Terminology D 1129.

### 4. Summary of Test Method

4.1 When a solution of p-dimethylaminobenzaldehyde in methyl alcohol and hydrochloric acid is added to hydrazine in diluted hydrochloric acid solution, a characteristic yellow color of p-dimethylaminobenzalazine is formed. The yellow color formed is proportional to the hydrazine present and is in good agreement with Beer's law in the range from 5.0 to 200  $\mu\text{g/L}$  (ppb) hydrazine.

### 5. Significance and Use

5.1 Hydrazine is a man-made chemical and is not found in natural waters. The determination of hydrazine is usually made on boiler feedwaters, process waters, and other waters that have been treated with hydrazine ( $N_2H_4$ ) for the purpose of maintaining residuals to prevent corrosion by dissolved oxygen. This reducing chemical reacts with dissolved oxygen to form nitrogen and water. However, under certain conditions it can also decompose to form ammonia and nitrogen. Hydrazine is used extensively as a preboiler treatment chemical for high-pressure boilers to scavenge small amounts of dissolved oxygen that are not removed by mechanical aeration. It has the advantage over sulfite treatment in that it does not produce any dissolved solids in the boiler water. Hydrazine is often determined in concentrations below 0.1 mg/L. However, in layup solutions for the protection of idle boilers, hydrazine may be present in concentrations as high as 200 mg/L.

5.2 Additionally, hydrazine provides protection to carbon steel by chemically reducing the unprotective layers of ferric oxide ( $Fe_2O_3$ ) to a more adherent protective layer of magnetite ( $Fe_3O_4$ ).

5.3 Hydrazine is a suspected carcinogen and a threshold limit value in the atmosphere of 1.0 mg/L has been set by OSHA. When in an aqueous solution, hydrazine will oxidize to nitrogen and water in the presence of air over a relatively short period of time.

### 6. Interferences

6.1 The substances normally present in industrial water do not interfere with the test; however, the hydrazine content may be diminished by oxidizing agents, such as chlorine, bromine, and iodine, collected with the sample or absorbed by it prior to testing.

6.2 Colors in the prescribed wavelengths also interfere, as do other dark colors or turbidities that cannot be overcome.

6.3 Aromatic amines, such as aniline, will also interfere.

## 7. Apparatus

7.1 *Photometer*—A spectrophotometer suitable for measurements at 458 nm and capable of holding cells with a light path of 50 mm should be used. Filter photometers and photometric practices prescribed in this test method shall conform to Practice E 60, and spectrophotometers to Practice E 275.

7.2 Certain photoelectric filter photometers are capable of measurement at 425 nm, but not at 458 nm. Measurements may be made at 425 nm with a reduction in sensitivity of approximately 50 % of that possible at 458 nm.

7.3 Instruments that read out in direct concentration can also be used. Manufacturer's instructions should be followed.

## 8. Reagents

8.1 *Purity of Reagents*—Reagent grade chemicals shall be used in all tests. Unless otherwise indicated, it is intended that all reagents shall conform to the specifications of the Committee on Analytical Reagents of the American Chemical Society, where such specifications are available.<sup>6</sup> Other grades may be used, provided it is first ascertained that the reagent is sufficiently high in purity to permit its use without lessening the accuracy of the determinations.

8.2 *Purity of Water*—Unless otherwise indicated, references to water shall be understood to mean Type II reagent water conforming to the requirements in Specification D 1193.

8.3 *Hydrazine Solution, Stock* (1.0 mL = 100 µg N<sub>2</sub>H<sub>4</sub>)—Dissolve 0.328 g of hydrazine dihydrochloride (HCl·NH<sub>2</sub>·NH<sub>2</sub>·HCl) in 100 mL of water and 10 mL of HCl (sp gr 1.19). Dilute with water to 1 L in a volumetric flask and mix (**Warning**, see Note 1).

8.4 *Hydrazine Solution, Standard* (1.0 mL = 0.500 µg N<sub>2</sub>H<sub>4</sub>)—Dilute 5.0 mL of hydrazine stock solution to 1 L with water and mix. Prepare as needed.

NOTE 1—**Warning:** Hydrazine is a suspected carcinogen and should be handled with care.<sup>7</sup>

8.5 *Hydrochloric Acid* (sp gr 1.19)—Concentrated hydrochloric acid (HCl).

8.6 *p-Dimethylaminobenzaldehyde Solution*—Dissolve 4.0 g of p-dimethylaminobenzaldehyde [(CH<sub>3</sub>)<sub>2</sub>NC<sub>6</sub>H<sub>4</sub>CHO] in 200 mL of methyl alcohol (CH<sub>3</sub>OH) and 20 mL of HCl (sp gr 1.19). Store in a dark bottle out of direct sunlight.

## 9. Sampling

9.1 Collect the sample in accordance with Practices 3370, Practice D 1066, or Specification D 1192, whichever is applicable (**Warning**, see Note 1).

9.2 Acidify and dilute the sample as soon as taken by adding 1 mL of concentrated HCl (sp gr 1.19) to a 100-mL volumetric

flask and then pipetting 50 mL of the sample into the flask and diluting to 100 mL. Prepare a blank with water at the same time.

9.3 A smaller sample aliquot should be taken if the hydrazine concentration is greater than 200 µg/L.

## 10. Calibration

10.1 Prepare a series of standard hydrazine solutions by pipetting 0.0, 5.0, 10.0, 25.0, 50.0, 100.0, and 200.0 mL of hydrazine standard solution (1.0 mL = 0.500 µg N<sub>2</sub>H<sub>4</sub>) into 500-mL volumetric flasks. Add 5 mL of HCl (sp gr 1.19) to each flask and dilute with water to 500 mL and mix well. This will give standard solutions containing 0, 5.0, 10.0, 25.0, 50.0, 100, and 200 µg/L (ppb) of hydrazine.

10.2 Pipet 50.0-mL portions of the hydrazine standard solutions into clean, dry 100-mL beakers or flasks and proceed as directed in 11.2. Plot absorbance on the ordinate and micrograms per litre of hydrazine on the abscissa of linear graph paper.

10.3 A separate calibration curve must be made for each photometer and a recalibration must be made if it is necessary to change the cell, lamp, or filter, or if any other alterations of instrument or reagents are made. Check the curve for each series of tests by running two or more solutions of known hydrazine concentrations.

## 11. Procedure

11.1 Pipet 50.0 mL of the blank, standard solutions, and acidified diluted sample solutions into clean, dry 100-mL beakers or flasks.

11.2 Add 10.0 mL of p-dimethylaminobenzaldehyde solution with a pipet to each beaker or flask and mix well.

11.3 After a minimum of 10 min, but no longer than 100 min, measure the color absorbance of each solution at 458 nm in a 50 mm cell with a spectrophotometer, using the blank as reference solution for the initial instrument setting at zero absorbance. The instrument may be calibrated with the standard solutions to read directly in concentration if such capabilities are available.

11.4 Determine the micrograms per litre of hydrazine by referring the absorbance obtained for the sample to the calibration curve or reading hydrazine concentration directly.

## 12. Calculation

12.1 Calculate the concentration of hydrazine in micrograms per litre (parts per billion) in the sample by applying the following equation for the hydrazine determined in 11.4:

$$\text{hydrazine (N}_2\text{H}_4\text{), } \mu\text{g/L (ppb)} = A \cdot B/C$$

where:

A = hydrazine indicated by the calibration curve or read directly from the instrument, µg/L,

B = volume of the flask, µg/L, in which the sample was diluted in Section 9.2, mL, and

C = volume of the sample, and taken in Section 9.2, mL.

<sup>6</sup> "Reagent Chemicals, American Chemical Society Specifications," Am. Chemical Soc., Washington, DC. For suggestions on the testing of reagents not listed by the American Chemical Society, see "Analar Standards for Laboratory Chemicals," BDH Ltd., Poole, Dorset, U.K., and the "United States Pharmacopeia."

<sup>7</sup> MacEwen, J. D., Vernot, E. H., Haun, C. C., and Kinkead, E. B., "Chronic Inhalation Toxicity of Hydrazine: Onconogenic Effects," in cooperation with the University of California (Irvine) and the Airforce Aero Medical Research Laboratory.

13. Precision and Bias <sup>8</sup>

13.1 The precision of this test method was tested by seven (7) laboratories in reagent water, condensate, well water, and natural water. Three laboratories reported data from two operators. Although multiple injections were reportedly made, the report sheets that were provided allowed only for reporting single values. Thus, no single operator precision can be calculated.

13.1.1 The overall precision of this test method, within its designated range for both reagent water and selected natural water matrices, varies with the quantity tested, as shown in Fig. 1.

13.1.2 Recovery and bias data for this test method are listed in Table 1.

TABLE 1 Recovery and Bias

Amount Added, µg/L	Amount Found, µg/L	% Bias	Statistically Significant, % (95 % Confidence Level)
Reagent Water Type II			
6.041	5.891	-2.5	No
51.57	51.54	-0.1	No
177.8	178.1	0.2	No
112.9	113.2	0.3	No
Selected Water Matrices			
6.041	5.935	-1.7	No
51.57	50.77	-1.6	No
177.8	176.2	-0.9	Yes
112.9	111.2	-1.5	No

13.2 These data may not apply to waters of other matrices; therefore, it is the responsibility of the analyst to ensure the validity of the test method in a particular matrix.

<sup>8</sup> Supporting data are available from ASTM Headquarters. Request RR: D19-1119.

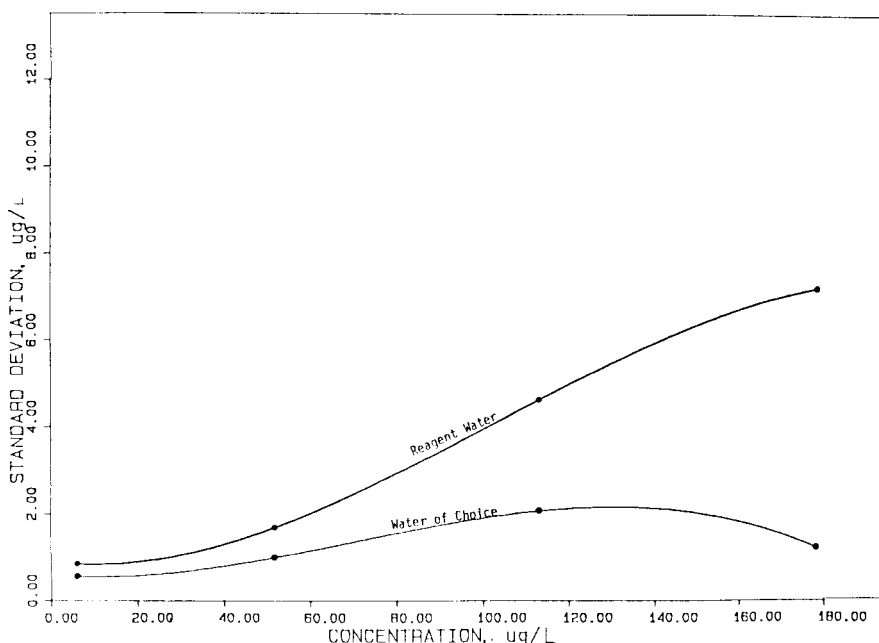


FIG. 1 Precision for Hydrazine

The American Society for Testing and Materials takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org).