



Designation: **D 3386 – 9400**

An American National Standard

Standard Test Method for Coefficient of Linear Thermal Expansion of Electrical Insulating Materials¹

This standard is issued under the fixed designation D 3386; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

This standard has been approved for use by agencies of the Department of Defense.

1. Scope

1.1 This test method covers determination of the coefficient of linear thermal expansion of electrical insulating materials by use of a thermomechanical analyzer.

1.2 This test method is applicable to materials that are solid over the entire range of temperature used, and that retain sufficient hardness and rigidity over the temperature range so that irreversible indentation of the specimen by the sensing probe does not occur.

1.3 Transition temperatures also may be obtained by this test method.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

1.5 The values stated in SI units are the standard.

NOTE 1—There is no similar or equivalent ISO/IEC standard.

2. Referenced Documents

2.1 *ASTM Standards:*

¹ This test method is under the jurisdiction of ASTM Committee ~~D-9~~ D09 on Electrical and Electronic Insulating Materials and is the direct responsibility of Subcommittee D09.01 on Electrical Insulating Varnishes, Powders, and Encapsulating Compounds.

Current edition approved ~~Oct. 15, 1994~~, Dec. 10, 2000. Published ~~December 1994~~, January 2001. Originally published as D 3386 – 84. Last previous edition ~~D 3386 – 84 (1989)~~—D 3386 – 94.

D 374M Test Methods for Thickness of Solid Electrical Insulation (Metric)²

~~D-618 Practice 696 Test Method for Conditioning Coefficient of Linear Thermal Expansion of Plastics Between – 30°C and Electrical Insulating Materials for Testing², 30°C³~~

~~D-696 Test Method 1711 Terminology Relating to Electrical Insulation²~~

~~D 6054 Practice for Coefficient of Linear Thermal Expansion of Plastics Between – 30°C and 30°C³ Coordinating Electrical Insulating Materials for Testing⁴~~

3. ~~Summary~~Terminology

~~3.1 See Terminology D 1711 for definitions of Test Method~~

~~3.1 This test method uses a thermomechanical analyzer other terms relating to determine the change of dimension as a function of temperature of a small specimen of a solid electrical insulating material. Coefficients of linear thermal expansion are calculated from the values. Other thermal observations may also be made. insulation.~~

4. ~~Significance and Use~~

~~4.1 Measurements Summary of coefficient of linear thermal expansion are useful in evaluating the suitability of solid insulating materials for use in combination with other materials where mechanical stresses may develop as a result of differences in coefficients.~~

~~4.2 This test method may be compared with Test Method D 696, but tests made with this Method~~

~~4.1 This test method use much smaller specimens. This eliminates the need for large liquid baths and greatly reduces the time required uses a thermomechanical analyzer to determine the change of dimension as a function of temperature equilibrium. As of a result, the time required for making small specimen of a test is less than for Test Method D 696, and solid electrical insulating material. Coefficients of linear thermal expansion are calculated from the test method can conveniently values. Other thermal observations may also be used over a wider temperature range than for Test Method D 696. made.~~

5. ~~Significance and Use~~

~~5.1 Measurements of coefficient of linear thermal expansion are useful in evaluating the suitability of solid insulating materials for use in combination with other materials where mechanical stresses may develop as a result of differences in coefficients.~~

~~5.2 This test method may be compared with Test Method D 696, but tests made with this test method use much smaller specimens. This eliminates the need for large liquid baths and greatly reduces the time required to reach temperature equilibrium. As a result, the time required for making a test is less than for Test Method D 696, and the test method can conveniently be used over a wider temperature range than for Test Method D 696.~~

6. ~~Apparatus~~

~~56.1 The thermomechanical analyzer shall include:~~

~~56.1.1 A specimen holder and probe, into which the specimen can be placed. Changes in height of the specimen are sensed by movement of the probe. Use a probe of a shape and size such that, for the material being tested, the load applied to the specimen by the probe shall not cause indentation of the specimen within the range of test temperatures of interest.~~

~~56.1.2 Means for sensing movement of the probe resulting from changes in height of the specimen and for translating these movements into a signal suitable for input to the recorder. The sensing element should be capable of sensing a change in height of 0.1 μm of the test specimen, with provisions for less sensitive ranges when needed.~~

~~56.1.3 Means for uniformly heating the specimen holder at a predetermined rate over the range of temperatures of interest. This will consist of a furnace and temperature controller with provisions for precooling the furnace and specimen holder when measurements of subambient temperatures are to be made.~~

~~56.1.4 Means for measuring temperature in immediate proximity to the test specimen.~~

~~56.1.5 Equipment for recording changes in specimen height as a function of specimen temperature.~~

~~56.1.6 Micrometer, meeting the requirements of Test Methods D 374M.~~

~~NOTE 1—Instruments from duPont TA Instruments and Perkin-Elmer have been found suitable.~~

6. ~~Test Specimens~~

~~6.1 Specimens shall be between 2.5 and 7.5 mm in height and shall have flat and parallel upper and lower surfaces. Lateral dimensions shall not exceed 10 mm.~~

7. ~~Calibration~~

~~7.1 Calibrate the apparatus Test Specimens~~

² Annual Book of ASTM Standards, Vol 10.01.

³ Annual Book of ASTM Standards, Vol 08.01.

⁴ Annual Book of ASTM Standards, Vol 10.02.

7.1 Specimens shall be between 2.5 and 7.5 mm in accordance with the instrument manufacturer's recommendations. height and shall have flat and parallel upper and lower surfaces. Lateral dimensions shall not exceed 10 mm.

8. Conditioning

8.1 Condition Calibration

8.1 Calibrate the test specimens for 1 h at 10°C above the maximum specified temperature of the run, followed by 40 h at the standard laboratory atmosphere apparatus in accordance with Practice D 618. the instrument manufacturer's recommendations.

9. Conditioning

9.1 Condition the test specimens for 1 h at 10°C above the maximum specified temperature of the run, followed by 40 h at the standard laboratory atmosphere in accordance with Practice D 6054.

10. Procedure

910.1 Measure the height of the specimen to within 0.01 mm.

910.2 Place the specimen in the specimen holder under the probe. Place the thermocouple or other means for sensing specimen temperature in contact with the specimen, or as near the specimen as possible.

910.3 Assemble the furnace to the specimen holder. If measurements at subambient temperatures are to be made, cool the specimen holder and furnace to at least 20°C below the lowest temperature of interest, using procedures as given by the instrument manufacturer. Do not allow the refrigerant used for cooling to come into direct contact with the specimen.

910.4 Increase the furnace temperature at $5 \pm 0.5^\circ\text{C}/\text{min}$ over the desired temperature range.

NOTE 23—A gas purge may be used to replace the air around the specimen for measurement of expansion in different atmospheres.

910.5 Record the specimen temperature and change in specimen height.

101. Calculation

101.1 Calculate the average coefficient of thermal expansion, α , over the temperature intervals of interest as follows:

$$\alpha = (\Delta H/\Delta T)/H \tag{1}$$

where:

H = original height of specimen,

ΔH = change in height of the specimen (in the same units) over the temperature interval ΔT , and

ΔT = temperature interval, °C (see Fig. 1).

NOTE 34— ΔH and ΔT may on some instruments be read directly from the recorder chart. On other instruments constant factors may need to be applied to the chart readings to obtain these values.

112. Report

112.1 Report the following information:

112.1.1 Designation of the material, including the name of the manufacturer and information on composition when known,

112.1.2 Method of preparation of the test specimen,

112.1.3 Specimen orientation with respect to original sample, if applicable,

112.1.4 Specimen height,

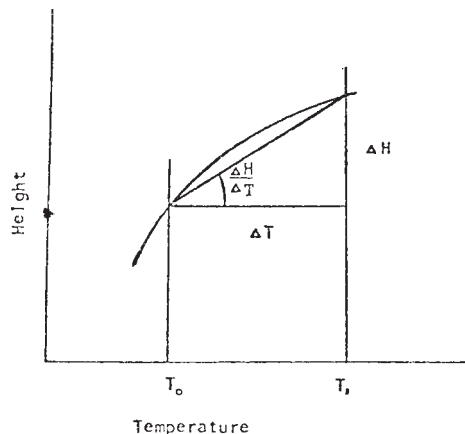


FIG. 1 Specimen Height versus Temperature

- 142.1.5 Temperatures between which the coefficient of linear thermal expansion has been determined,
- 142.1.6 Average coefficient of linear thermal expansion per degree Celsius,
- 142.1.7 Transition temperatures, if noted,
- 142.1.8 Instrument manufacturer and model number,
- 142.1.9 Purge gas, if used, and rate of gas flow, and
- 142.1.10 X-Y chart record.

12. Precision and Bias

- 12.1 The precision of this test method has not been determined.
- 12.2 Operators familiar with this test method estimate that individual values may vary from the mean value by as much as 25 %, both within a given laboratory and between laboratories. By closely controlling both the dimensions and the orientation of the test specimens, better reproducibility has been achieved.
- 12.3 The bias of this test method has not been determined.

13. Precision and Bias

- 13.1 The precision of this test method has not been determined.
- 13.2 Operators familiar with this test method estimate that individual values may vary from the mean value by as much as 25 %, both within a given laboratory and between laboratories. By closely controlling both the dimensions and the orientation of the test specimens, better reproducibility has been achieved.
- 13.3 The bias of this test method has not been determined.

14. Keywords

- 14.1 linear thermal expansion; thermomechanical analyzer; transition temperature

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org).