

This document is not an ASTM standard and is intended only to provide the user of an ASTM standard an indication of what changes have been made to the previous version. Because it may not be technically possible to adequately depict all changes accurately, ASTM recommends that users consult prior editions as appropriate. In all cases only the current version of the standard as published by ASTM is to be considered the official document.



---

**Designation: D 1783 – 91 (Reapproved 1995)**


**Designation: D 1783 – 01**

# Standard Test Methods for Phenolic Compounds in Water<sup>1</sup>

This standard is issued under the fixed designation D 1783; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ε) indicates an editorial change since the last revision or reapproval.

*This standard has been approved for use by agencies of the Department of Defense.*

<sup>1</sup> These test methods are under the jurisdiction of D-19 on Water and are the direct responsibility of Subcommittee D19.06 on Methods for Analysis for Organic Substances in Water.

Current edition approved ~~Sept. 15, 1991~~; Feb. 10, 2001. Published ~~December 1991~~; May 2001. Originally published as D 1783 – 60 T. Last previous edition D 1783 – 8791 (1995).

## 1. Scope

1.1 These test methods cover the preparation of the sample and the determination of the concentration of phenolic compounds in water. They are based on the color reaction of phenol (C<sub>6</sub>H<sub>5</sub>OH) with 4-aminoantipyrine and any color produced by the reaction of other phenolic compounds is reported as phenol. The concentration of phenol measured represents the minimum concentration of phenolic compounds present in the sample.

1.2 Phenolic compounds with a substituent in the para position may not quantitatively produce color with 4-aminoantipyrine. However, para substituents of phenol such as carboxyl, halogen, hydroxyl, methoxyl, or sulfonic acid groups do produce color with 4-aminoantipyrine.

1.3 These test methods address specific applications as follows:

	Range	Sections
Test Method A—Chloroform Extraction	0 to 100 µg/L	11 to 17
Test Method B—Direct Photometric	>0.1 mg/L (100 µg/L)	18 to 24

1.4 It is the users' responsibility to assure the validity of the standard test method for use in their particular matrix of interest.

1.5 *This standard does not purport to address all the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.* For specific hazard statements see Note 1 and Note 3.

## 2. Referenced Documents

### 2.1 ASTM Standards:

D 1129 Terminology Relating to Water<sup>2</sup>

D 1192 Specification for Equipment for Sampling Water and Steam in Closed Conduits<sup>2</sup>

D 1193 Specification for Reagent Water<sup>2</sup>

D 1293 Test Methods for pH of Water<sup>2</sup>

D 2777 Practice for Determination of Precision and Bias of Applicable Methods of Committee D-19 on Water<sup>2</sup>

D 3370 Practices for Sampling Water from Closed Conduits<sup>2</sup>

D 5789 Writing Quality Control Specifications for Standard Test Methods for Organic Constituents<sup>2</sup>

D 5810 Guide for Spiking Into Aqueous Samples<sup>2</sup>

D 5847 Practice for Writing Quality Control Specifications for Standard Test Methods for Water Analysis<sup>2</sup>

## 3. Terminology

3.1 *Definitions*—For definitions of terms used in these test methods, refer to Terminology D 1129.

3.2 *Definitions of Terms Specific to This Standard:*

3.2.1 *phenolic compounds*—hydroxy derivatives of benzene and its condensed nuclei.

## 4. Summary of Test Methods

4.1 Test Methods A and B are photometric procedures based on the reaction of steam-distillable phenolic compounds with 4-aminoantipyrine.

<sup>2</sup> Annual Book of ASTM Standards, Vol 11.01.

4.2 Test Method A differs from B mainly in that the sample is extracted with chloroform, thereby providing 20-fold greater sensitivity.

4.3 Both procedures involve first separating the phenolic compounds from the background matrix by distillation. Due to the differing solubilities and boiling points of the various phenolic compounds, each phenolic comes over in the distillation at a different rate. Some phenolics will be substantially transferred near the beginning of the distillation and some will not start to distill until near the end. For this reason some phenolics may not have been quantitatively transferred to the receiving flask when the specified volume of distillate has been collected.

## 5. Significance and Use

5.1 Phenolic compounds are sometimes found in surface waters from natural and industrial sources. Their presence in streams and other waterways frequently will cause off flavor in fish tissue and other aquatic food.

5.2 Chlorination of waters containing phenols may produce chlorophenols that are odoriferous and objectionable tasting.

## 6. Interferences

6.1 Common interferences that may occur in waters are phenol-decomposing bacteria, reducing substances, and strongly alkaline conditions of the sample. Provisions incorporated in these test methods will minimize the effects of such interferences.

6.2 Treatment procedures required prior to the analysis for removal of interfering compounds may result in the unavoidable elimination or loss of certain types of phenolic compounds. It is beyond the scope of these test methods to describe procedures for overcoming all of the possible interferences that may be encountered in the test methods, particularly with highly contaminated water and industrial waste water. The procedures used must be revised to meet the specific requirements.

6.3 A few methods for eliminating certain interferences are suggested. (See Section 8 for descriptions of reagents required.)

6.3.1 *Oxidizing Agents*—If the sample smells of chlorine, or if iodine is liberated from potassium iodide on acidification of the sample, remove the oxidizing agents so indicated immediately after sampling. The presence of oxidizing agents in the sample may oxidize some or all of the phenols in a short time. Ferrous sulfate or sodium arsenite solution may be added to destroy all of the oxidizing substances. Excess ferrous sulfate or sodium arsenite do not interfere since they are removed in the distillation procedure.

6.3.2 *Sulfur Compounds*—Compounds that liberate hydrogen sulfide ( $H_2S$ ) or sulfur dioxide ( $SO_2$ ) on acidification may interfere with the phenol determination. Treatment of the acidified sample with copper sulfate usually eliminates such interferences. Acidify the sample with sulfuric acid ( $H_2SO_4$ ) or hydrochloric acid ( $HCl$ ) until just acid to methyl orange. Then add a sufficient quantity of copper sulfate ( $CuSO_4$ ) solution to give a light blue color to the sample or until no more copper sulfide ( $CuS$ ) precipitate is formed. Excessive amounts of  $H_2S$  or  $SO_2$  may be removed from the acidified sample by a brief aeration treatment or stirring before the addition of the  $CuSO_4$  solution or both.

NOTE 1—**Warning:** Acidification of certain samples may produce vigorous evolution of carbon dioxide ( $CO_2$ ),  $SO_2$ ,  $H_2S$ , or other gases. Therefore, perform the acidification cautiously and stir the samples during the process. Complete the evolution of gases before the sample is stoppered.

6.3.3 *Oils and Tars*—If the sample contains oil or tar, some phenolic compounds may be dissolved in these materials. An alkaline extraction, in the absence of  $CuSO_4$  (Note 1), may be used to eliminate the tar and oil. Adjust the pH of the sample between 12 and 12.5 with sodium hydroxide ( $NaOH$ ) pellets to avoid extraction of the phenols. Extract the mixture with carbon tetrachloride ( $CCl_4$ ). Discard the oil- or tar-containing layer. Remove any  $CCl_4$  remaining in the aqueous portion of the sample by gentle heating.

NOTE 2—The presence of  $CuSO_4$  is detrimental since it is converted to cupric hydroxide ( $Cu(OH)_2$ ) by the  $NaOH$ . The  $Cu(OH)_2$  acts as an oxidizing agent on phenols.

## 7. Apparatus

7.1 *Buchner-Type Funnel with Coarse Fritted Disk*—At least three funnels are needed for determination of phenolic compounds by Test Method A. Alternatively, standard glass funnels and pre-fluted filter paper may be used. The funnel paper must be large enough to hold 5 g of sodium sulfate. These funnels are not used in Test Method B.

7.2 *Photometer*—A spectrophotometer or filter photometer, suitable for use at 460 nm (Test Method A) or at 510 nm (Test Method B), and accommodating a cell that gives a light path of 1.0 to 10 cm shall be used. The size of the cell used will depend on the absorbance of the colored solutions being measured and the characteristics of the photometer. In general, if the absorbances are greater than 1.0 with a larger cell, the next smaller size cell should be used.

7.3 *Distillation Apparatus*—A 1-L, heat-resistant, distilling flask attached to a Graham condenser by means of a glass joint.

7.4 *pH Meter*—This apparatus shall conform to the requirements in Test Methods D 1293.

## 8. Reagents

NOTE 3—**Warning:** Phenol, carbon tetrachloride, and chloroform are potentially hazardous to human health. **Caution**—Avoid inhalation and direct contact. Use in a well-ventilated hood.

8.1 *Purity of Reagents*—Reagent grade chemicals shall be used in all tests. Unless otherwise indicated, it is intended that all reagents shall conform to the specifications of the Committee on Analytical Reagents of the American Chemical Society, where

such specifications are available.<sup>3</sup> Other grades may be used, provided it is first ascertained that the reagent is of sufficiently high purity to permit its use without lessening the accuracy of the determination.

8.2 *Purity of Water*—Unless otherwise indicated, references to water shall be understood to mean water conforming to Specification D 1193 Types I, II, III, or IV. Water used for these test methods shall be free of phenolic compounds, residual chlorine, and substances that interfere with the test. Water sufficiently free of phenolics can be generated by boiling the water for 20 minutes.

8.3 *Aminoantipyrine Solution (20 g/L)*—Dissolve 2.0 g of 4-aminoantipyrine in water and dilute to 100 mL. Prepare this reagent fresh as used.

NOTE 4—The melting point of a satisfactory grade of 4-aminoantipyrine ranges from 108.0 to 109.5°C.

8.4 *Ammonium Chloride Solution (20 g/L)*—Dissolve 20 g of ammonium chloride (NH<sub>4</sub>Cl) in water and dilute to 1 L.

8.5 *Ammonium Hydroxide (NH<sub>4</sub>OH)* (sp gr 0.90)—Concentrated ammonium hydroxide (NH<sub>4</sub>OH).

8.6 *Carbon Tetrachloride (CCl<sub>4</sub>)*.

8.7 *Chloroform (CHCl<sub>3</sub>)*.

8.8 *Hydrochloric Acid (HCl)* (sp gr 1.19)—Concentrated hydrochloric acid (HCl).

8.9 *Phenol Solution, Stock* (1 mL = 10 mg phenol)—Dissolve 1.00 g of phenol (C<sub>6</sub>H<sub>5</sub>OH) in freshly boiled and cooled water. Dilute to 1 000 mL with freshly boiled cooled water. Prepare a fresh stock solution within 30 days of use.

8.10 *Phenol Solution, Intermediate*—(C<sub>6</sub>H<sub>5</sub>OH) (1 mL = 10 µg phenol)—Dilute 10.0 mL of the stock solution to 1 000 mL with freshly boiled and cooled water. Prepare this solution fresh on the day it is used.

8.11 *Phenol Solution, Standard* —(C<sub>6</sub>H<sub>5</sub>OH) (1 mL = 1.0 µg phenol)—Dilute 50 mL of the intermediate solution to 500 mL with freshly boiled and cooled water. Prepare this solution fresh within 2 h of use.

8.12 *Potassium Ferricyanide Solution (K<sub>3</sub>Fe(CN)<sub>6</sub>) (80 g/L)*—Dissolve 8.0 g of (K<sub>3</sub>Fe(CN)<sub>6</sub>) in water and dilute to 100 mL. Filter if necessary. Prepare fresh weekly.

8.13 *Sodium Bisulfate (NaHSO<sub>4</sub>)*.

8.14 *Sodium Sulfate (Na<sub>2</sub>SO<sub>4</sub>)*, anhydrous and granular.

8.15 *Sulfuric Acid (H<sub>2</sub>SO<sub>4</sub>)* (sp gr 1.84)—Concentrated sulfuric acid (H<sub>2</sub>SO<sub>4</sub>).

8.16 *Sulfuric Acid Solution (H<sub>2</sub>SO<sub>4</sub>) (1 + 9)*—Cautiously add one volume of concentrated H<sub>2</sub>SO<sub>4</sub> to nine volumes of water with continuous cooling and mixing. Solution will become hot.

## 9. Sampling

9.1 Collect the sample in accordance with Specification D 1192 and Practices D 3370.

9.2 When samples are composited, chill the samples or the composite sample immediately and keep at a temperature of not more than 4°C during the compositing period. The collection time for a single composite sample shall not exceed 4 h. If longer sampling periods are necessary, collect a series of composite samples. Then preserve such composite samples in accordance with Section 10 until analyzed.

## 10. Preservation of Samples

10.1 Phenolic compounds in water are subject to both chemical and biochemical oxidation. Preserve samples within 4 h of collection. Acidify the samples to a pH between 0.5 and 2.0 with H<sub>3</sub>PO<sub>4</sub>, HCl, H<sub>2</sub>SO<sub>4</sub>, or NaHSO<sub>4</sub>.

10.2 To further minimize any changes in the phenolic content of the sample, keep it cold, preferably between 2°C and 4°C until analysis. The preserved samples should be in glass, not plastic bottles, and preferably analyzed within 28 days after collection.

## TEST METHOD A—CHLOROFORM EXTRACTION

### 11. Scope

11.1 This test method is generally applicable to water that contains less than 100 µg/L (0.1 mg/L) of phenolic compounds. Lower levels may be achieved with different instruments and larger cells. Higher levels can be achieved by dilution.

11.2 The lowest levels of analyte detection or accurate quantitation are laboratory and sample matrix dependent and it is up to the users of the test method to determine these levels in their own situation.

11.3 This test method was tested on municipal wastewater treatment plant influent and effluent, lake water, river water, and industrial treatment plant effluent. It is the user's responsibility to insure the validity of this test method for waters of untested matrices.

### 12. Summary of Test Method

12.1 This is a photometric test method, based on the reaction of steam-distillable phenolic compounds with 4-aminoantipyrine at a pH of 10.0 ± 0.2 in the presence of K<sub>3</sub>Fe(CN)<sub>6</sub>. The antipyrine dye formed is extracted from the aqueous solution with

<sup>3</sup> *Reagent Chemicals, American Chemical Society Specifications*, American Chemical Society, Washington, DC. For suggestions on the testing of reagents not listed by the American Chemical Society, see *Analar Standards for Laboratory Chemicals*, BDH Ltd., Poole, Dorset, U.K., and the *United States Pharmacopeia and National Formulary*, U.S. Pharmaceutical Convention, Inc. (USPC), Rockville, MD.

chloroform and the absorbance is measured at 460 nm. The concentration of phenolic compounds in the sample is expressed in terms of micrograms per litre of phenol C<sub>6</sub>H<sub>5</sub>OH.

### 13. Calibration

13.1 Prepare a series of 500-mL C<sub>6</sub>H<sub>5</sub>OH standards in freshly boiled and cooled water containing 0, 5, 10, 20, 30, 40, and 50 mL of standard C<sub>6</sub>H<sub>5</sub>OH solution (1 mL = 1.0 µg C<sub>6</sub>H<sub>5</sub>OH). Use all solutions at room temperature.

13.2 Develop color in the series of standards and prepare the chloroform extracts in accordance with the procedures prescribed in Section 14 and 15.

13.3 Measure the absorbance of each standard at 460 nm against the reagent blank as zero absorbance. Plot the absorbances against the corresponding weights in micrograms of phenol.

NOTE 5—Make a separate calibration curve for each spectrophotometer or photoelectric colorimeter. Check each curve periodically to ensure reproducibility.

### 14. Distillation Procedure

14.1 Measure 500 mL of the sample into a beaker. Adjust the pH of the sample to between pH 0.5 and 4 with H<sub>2</sub>SO<sub>4</sub> solution (1 + 9). Use methyl orange indicator solution or a pH meter to aid in the pH adjustment. If the sample has been previously preserved according to 10.1, this pH adjustment step may be omitted. Transfer the mixture to the distillation apparatus. Use a 500-mL graduated cylinder as a receiver.

14.2 Distill 450 mL of the sample. Stop the distillation and, when boiling ceases, add 50 mL of water to the distillation flask. Continue the distillation until a total of 500 mL has been collected.

14.3 If the distillate is turbid, a second distillation may prove helpful. Acidify the turbid distillate with H<sub>2</sub>SO<sub>4</sub> solution (1 + 9) and repeat the previously described distillation. The second distillation usually eliminates the turbidity. However, if the second distillate is also turbid, the screening procedure must be modified. Attempt an extraction process before the distillation to avoid turbidity in the distillate.

### 15. Determination of Phenolic Compounds

15.1 Transfer to a beaker the 500 mL of distillate, or a suitable aliquot diluted to 500 mL containing no more than 50 µg of phenolic compounds. The distillate and all solutions used must be at room temperature. Trial and error tests may be necessary to determine the volume of a suitable aliquot. Also, prepare a blank consisting of 500 mL of water.

15.2 Add 25 mL of NH<sub>4</sub>Cl solution to each aliquot. Adjust the pH between 9.8 and 10.2 with NH<sub>4</sub>OH. Transfer each mixture to a 1-L separatory funnel. Add 3.0 mL of 4-aminoantipyrine solution (20 g/L) and mix immediately, then add 3.0 mL of K<sub>3</sub>Fe(CN)<sub>6</sub> solution and again mix immediately. Allow color to develop for 3 min.

NOTE 6—The solutions should be clear and have a light yellow color. If not, an interfering substance is indicated. Repeat the determination after more complete treatment to eliminate the interference.

15.3 Pipet 25.0 mL of chloroform into each separatory funnel if a 1.0 to 5.0-cm cell is to be used in the colorimeter. Add 50.0 mL if a 10-cm cell is to be used. Shake the separatory funnel ten times. When the chloroform has settled, again shake the separatory funnel ten times and allow the chloroform to settle.

15.4 Filter each of the chloroform extracts through separate fritted-glass funnels or fluted filter paper in standard funnels containing 5 g of anhydrous, granular Na<sub>2</sub>SO<sub>4</sub> directly into clean absorption cells as needed for absorbance measurements. Do not add additional chloroform.

15.5 Using the chloroform extract of the reagent blank adjust the colorimeter to zero absorbance at 460 nm. Measure the absorbance of the sample extract at the same wavelength. By reference to the calibration curve (Section 13) and the absorbance obtained on the sample extract, determine the phenolic content of the sample.

### 16. Calculation

16.1 Calculate the phenolic content of the sample, in micrograms per litre, as follows:

$$\text{Concentration of phenolics in original sample } \mu\text{g/L} = W \times 100/V$$

where:

$W$  = phenolics, in aliquot of sample distillate diluted to 500 mL as determined from calibration curve, µg, and

$V$  = sample distillate, in the 500-mL solution reacted with 4-aminoantipyrine, mL.

NOTE 7—Since the ratio of the various phenolic compounds present in a given sample is unpredictable, phenol (C<sub>6</sub>H<sub>5</sub>OH) is used as a standard. Any color produced by the reaction of other phenolic compounds is reported as phenol. This value will represent the minimum concentration of phenolic compounds present in the sample.

## 17. Precision and Bias <sup>4</sup>

17.1 Eight laboratories participated in a collaborative study to determine the precision and bias of this procedure. The study was conducted by sending C<sub>6</sub>H<sub>5</sub>OH concentrates to participating laboratories. The laboratories then spiked these concentrates into phenol free reagent grade water and an optional water matrix of their choice. The precision and bias values determined in this study include any variability due to make up, splitting, shipment, and dilution of the concentrates used.

17.2 The optional water matrices chosen by the participants included: river water (2), municipal wastewater treatment plant effluent (3), lake water (1), raw sewage (1), and industrial wastewater treatment plant effluent (1). All of the data from the optional matrix portion of the study was combined to obtain composite precision values. None of the matrices used seemed to have a greater effect on precision than any other, but they did have the effect of degrading recovery (bias). The precision on samples in the optional matrix was comparable to that obtained with the reagent water matrix.

17.3 The collaborative study and data analysis was performed using Practice D 2777. Within each matrix, each laboratory analyzed three concentration levels, each in triplicate.

17.4 The final precision data are summarized in Table 1,

where:

$S_T$  = between laboratory standard deviation, and

$S_O$  = within laboratory standard deviation from geometric mean of weighted individual laboratory variances).

The precision of this test method depends in part on the interferences present and the skill of the analyst.

17.5 The bias of the test method, as indicated from the collaborative study, is summarized in Table 2. This data is displayed graphically in Fig. 1 and Fig. 2.

17.6 ~~The quality assurance/quality control (QA/QC) portion of this test method has not been completely established at this time. It is the intent of the ASTM Subcommittee responsible for this test method, that procedures be incorporated into this test method that require a minimum level of QC. These procedures will require at a minimum, a method start-up check and ongoing performance checks. The analysts performing this test method will be required to measure their performance against the performance level achieved by the laboratories that participated in the ASTM round-robin study done on this test method. These formal QC procedures will be incorporated at such a time as they have been officially accepted by the ASTM.~~

## TEST METHOD B—DIRECT PHOTOMETRIC

### 18. Scope

18.1 This test method is applicable to water that contains more than 0.1 mg/L of phenolic compounds.

NOTE 8—Some laboratories have reported being able to measure concentrations as low as 0.005 mg/L using 10-cm absorption cells.

18.2 The lowest levels of analyte detection or accurate quantitation is laboratory and sample matrix dependent and it is up to the users of the test method to determine these levels in their own situation.

18.3 This test method was tested on municipal wastewater treatment plant influent and effluent, river water, lake water, tap water, and industrial treatment plant effluent. It is the user's responsibility to ensure the validity of this test method for waters of untested matrices.

### 19. Summary of Test Method

19.1 This is a photometric test method, based on the reaction of steam-distillable phenolic compounds with 4-aminoantipyrine at a pH of 10.0 ± 0.2 in the presence of K<sub>3</sub>Fe(CN)<sub>6</sub>. The antipyrine color formed in a aqueous solution is measured at 510 nm. The concentration of phenolic compounds in the sample is expressed in terms of milligrams per litre of phenol (C<sub>6</sub>H<sub>5</sub>OH).

### 20. Calibration

20.1 Prepare a series of 100-mL phenol standards in water containing 0, 10, 20, 30, 40 and 50 mL of intermediate standard phenol solution (1 mL = 0.01 mg phenol). Use all solutions at room temperature.

<sup>4</sup> Supporting data are available from ASTM Headquarters. Request RR: D19- 1132.


**TABLE 1 Precision Data—Test Method A**

Level	Reagent Water Matrix			Optional Water Matrix		
	6.460 µg/L	34.780 µg/L	67.900 µg/L	5.430 µg/L	32.840 µg/L	66.260 µg/L
n	23	23	23	24	24	23
$S_T$	3.384	4.190	8.923	2.494	3.957	8.147
$S_O$	2.718	5.320	7.300	2.528	3.243	5.850
$S_o:C.V.$ <sup>A</sup>	38%	10.8 %	11.8%	46.6 %	9.9%	8.8 %

<sup>A</sup> Coefficient of variation ( $S_o$  level) by 100.

**TABLE 2 Bias Data—Test Method A**

Reagent Water Matrix				
Amount Added, $\mu\text{g/L}$	Amount Found, $\mu\text{g/L}$	$\pm$ Bias, $\mu\text{g/L}$	$\pm$ Bias, %	Statistically Significant
7.154	6.460	-0.693	-9.7	no
35.768	34.780	-0.990	-2.8	no
71.535	67.900	-3.631	-5.1	no
Optional Water Matrix				
Amount Added, $\mu\text{g/L}$	Amount Found, $\mu\text{g/L}$	$\pm$ Bias, $\mu\text{g/L}$	$\pm$ Bias, %	Statistically Significant
7.154	5.430	-1.729	-24.0	yes
35.768	32.840	-2.930	-8.2	yes
71.535	66.260	-5.274	-7.4	yes

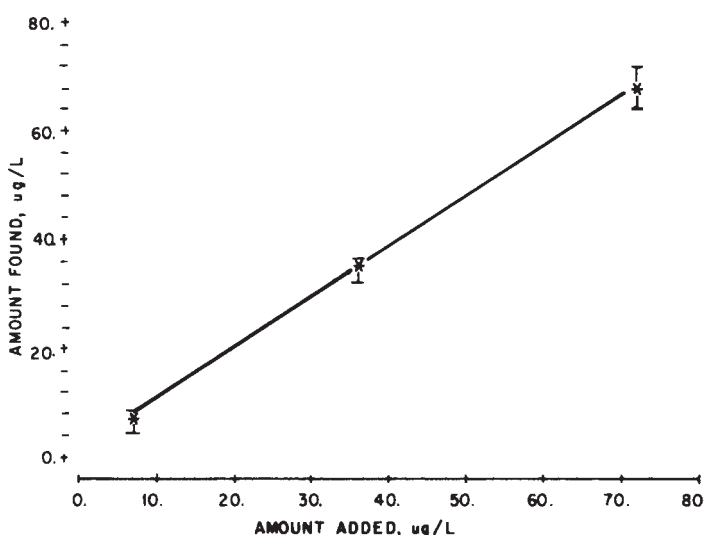

**FIG. 1 Plot of Amount Added Versus Amount of Phenol Found in Reagent Water**

20.2 Develop color in the series of standards in accordance with the procedure prescribed in Section 22.

20.3 Measure the absorbance of each standard at 510 nm against the reagent blank as zero absorbance. Plot the absorbances against the corresponding weight in milligrams of phenol (Note 5).

## 21. Distillation Procedure

21.1 See Section 14.

NOTE 9—Some laboratories have reported distilling only 100 mL of sample (and collecting 100 mL of distillate) with good success. This allows reducing the distillation time to 1/5 of that usually required. To distill the smaller volume of sample, the distillation equipment, the reagent addition and the water addition should be scaled down proportionately.

## 22. Determination of Phenolic Compounds

22.1 Transfer to a beaker 100 mL of distillate, or a suitable aliquot diluted to 100 mL containing no more than 0.50 mg of phenolic compounds. Use the distillate and all solutions at room temperature. Trial and error tests may be necessary to determine the volume of a suitable aliquot. Also, prepare a blank consisting of 100 mL of water.

22.2 Add 5 mL of  $\text{NH}_4\text{Cl}$  solution to each. Adjust the pH between 9.8 and 10.2 with  $\text{NH}_4\text{OH}$ . Add 2.0 mL of 4-aminoantipyrine solution, mix immediately, then add 2.0 mL of  $\text{K}_3\text{Fe}(\text{CN})_6$  solution and again mix immediately.

22.3 After 15 min, transfer the solutions to absorption cells and measure the absorbance of the sample solution against the zero absorbance of the reagent blank of 510 nm. By reference to the calibration curve (Section 20) and the absorbance obtained on the sample solution, determine the phenolic content of the sample.

## 23. Calculation

23.1 Calculate the phenolic content of the sample, in milligrams per litre, as follows:

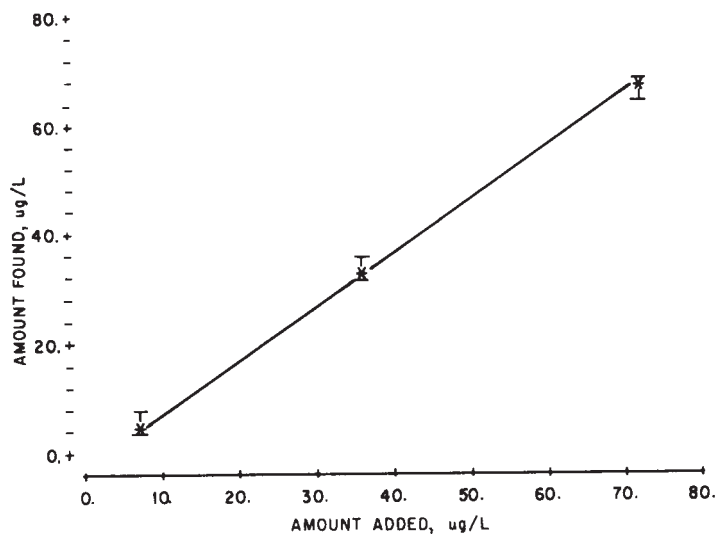


FIG. 2 Plot of Amount Added Versus Amount of Phenol Found in Optional Matrix

$$\text{Concentration of phenolic in original sample mg/L} = W \times 1000/V$$

where:

$W$  = phenolics, in aliquot of sample diluted to 100 mL, as determined from calibration curve, mg,

$V$  = original sample, present in 100 mL of the solution reacted with 4-aminoantipyrine, mL.

#### 24. Precision and Bias <sup>4</sup>

24.1 Nine laboratories participated in a collaborate study to determine the precision and bias of this procedure. The study was conducted by sending phenol concentrates to participating laboratories. The laboratories then spiked these concentrates into phenol free reagent grade water or an optional water matrix of their choice. The precision and bias values determined in this study include any variability due to make up, splitting, shipment, and dilution of the concentrates used.

24.2 The optional background water matrices chosen by the participants included: saline industrial waste (1), river water (1), municipal wastewater treatment plant effluent (3), lake water (1), raw sewage (1), tap water (1), and industrial wastewater treatment plant effluent (1). No one of the matrices used seemed to have a greater effect on the precision or bias of the results than any other. Precision and bias between the reagent water and optional matrix samples was comparable.

24.3 The collaborative study and data analysis was performed using Practice D 2777. Within each matrix, each laboratory analyzed three concentration levels, each in triplicate.

24.4 The final precision data are summarized in Table 3,

where:

$S_T$  = between laboratory standard deviation, and

$S_O$  = within laboratory standard deviation (from mean of geometrically weighted individual laboratory variances).

$S_T$  and  $S_O$  in reagent water varied approximately linearly with measured concentration range studied according to the following equations:

$$S_T = -0.056 + 0.039X \quad r^2 = 100.0 \%$$

$$S_O = -0.094 + 0.036X \quad r^2 = 98.2 \%$$

where:

TABLE 3 Precision Data—Test Method B

Level	Reagent Water Matrix			Optional Water Matrix		
	6.930 mg/L	34.430 mg/L	68.780 mg/L	6.960 mg/L	34.240 mg/L	68.940 mg/L
n	27	27	26	26	26	26
$S_T$	0.228	1.274	2.653	0.411	1.113	3.152
$S_O$	0.226	1.035	2.460	0.337	1.080	2.460
So:C.V. <sup>A</sup>	3.3 %	3.0 %	3.5%	4.7 %	3.1 %	3.5 %

<sup>A</sup> Coefficient of variation ( $S_O$  level) by 100.

X is the concentration level of phenol measured in the sample. The precision of this test method depends in part on the interferences present and the skill of the analyst.

24.5 The bias of this test method, as indicated from the collaborative study, is summarized in Table 4. This data is displayed graphically in Fig. 3 and Fig. 4.

24.6 The quality assurance/quality control (QA/QC) portion of this test method has not been completely established at this time. It is the intent of the ASTM subcommittee responsible for this test method that procedures be incorporated into this method requiring a minimum level of QC. These procedures will require at a minimum, a method of start-up check and ongoing performance checks. The analysts performing this test method will be required to measure their performance against the performance level achieved by the laboratories that participated in the ASTM round-robin study done on this test method. These formal QC procedures will be incorporated at such time as they have been officially accepted by ASTM.

## 25. Quality Control

25.1 In order to be certain that analytical values obtained using this test method are valid and accurate within the confidence limits of the test, the following QC procedures must be followed when running the test:

### 25.2 Calibration and Calibration Verification

#### 25.2.1 Instrument

25.2.1.1 A calibration curve must be prepared as specified in Methods A and B prior to analysis of samples to calibrate the instrument.

25.2.1.2 Verify the instrument calibration each day before use by analyzing a standard at the mid-range concentration of the method.

25.2.1.3 If the calibration check fails, check for and resolve any spectrophotometer problems and recalibrate the instrument.

### 25.3 Initial Demonstration of Laboratory Capability

25.3.1 If a laboratory has not performed the test before or there has been a major change in the measurement system, for example new analyst, new instrument, etc., a precision and bias study must be performed to demonstrate laboratory capability.

25.3.2 Analyze seven replicates of a standard solution prepared from an IRM containing C<sub>6</sub>H<sub>5</sub>OH at 30 µg/L for Method A or 30 mg/L for Method B. The matrix and chemistry of the solution should be equivalent to the solution used in the collaborative study. Each replicate must be taken through the complete analytical test method including any sample preservation and pretreatment steps. The replicates may be interspersed with samples.

25.3.3 Calculate the mean and standard deviation of the seven values and compare to the acceptable ranges of precision and bias in Table 5. If concentration other than those specified in 25.3.2 are used, follow procedures in D 5789 and D 5847 to determine acceptable ranges of precision and bias.

### 25.4 Laboratory Control Sample

25.4.1 To ensure that the test method is in control, analyze an LCS containing C<sub>6</sub>H<sub>5</sub>OH of 30 µg/L for Method A or 30 mg/L for Method B with each batch of samples. The LCS must be taken through all of the steps of the analytical method including sample preservation and pretreatment. The results obtained for the LCS shall fall within the limits in Table 5. If concentrations other than those specified above are used, follow procedures in D 5789 and D 5847 to determine acceptable recovery.

25.4.2 If the result is not within these limits, analysis of samples is halted until the problem is corrected, and either all samples in the batch must be reanalyzed, or the results must be qualified with an indication that they do not fall within the performance criteria of the test method.

### 25.5 Method Blank (Blank)

25.5.1 Analyze a reagent water test blank with each batch. The concentration of C<sub>6</sub>H<sub>5</sub>OH must be less than the method detection limit for each method. If the concentration of C<sub>6</sub>H<sub>5</sub>OH is found above the level, analysis of samples is halted until the

**TABLE 4 Bias Data—Test Method B**

Reagent Water Matrix				
Amount Added, mg/L	Amount Found, mg/L	±Bias, mg/L	±Bias, %	Statistically Significant
7.154	6.930	-0.224	-3.1	yes
35.768	34.430	-1.338	-3.7	yes
71.535	68.777	-2.758	-3.9	yes
Optional Water Matrix				
Amount Added, mg/L	Amount Found, mg/L	±Bias, mg/L	±Bias, %	Statistically Significant
7.154	6.958	-0.196	-2.7	yes
35.768	34.242	-1.526	-4.3	yes
71.535	68.942	-2.593	-3.6	yes

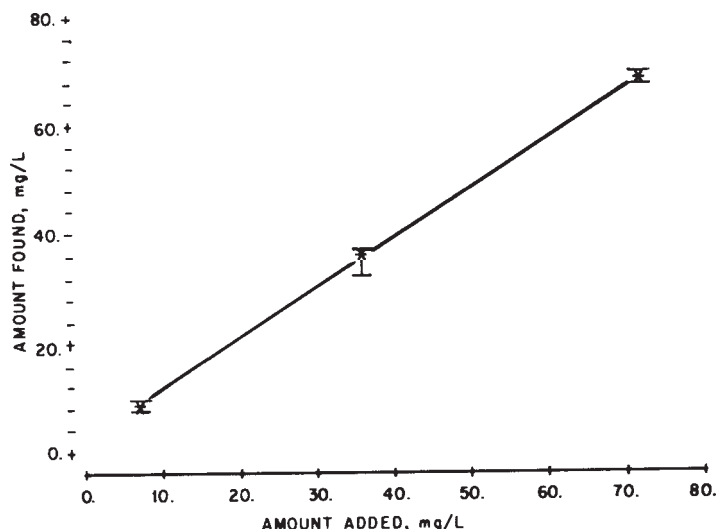


FIG. 3 Plot of Amount Added Versus Amount of Phenol Found in Reagent Water

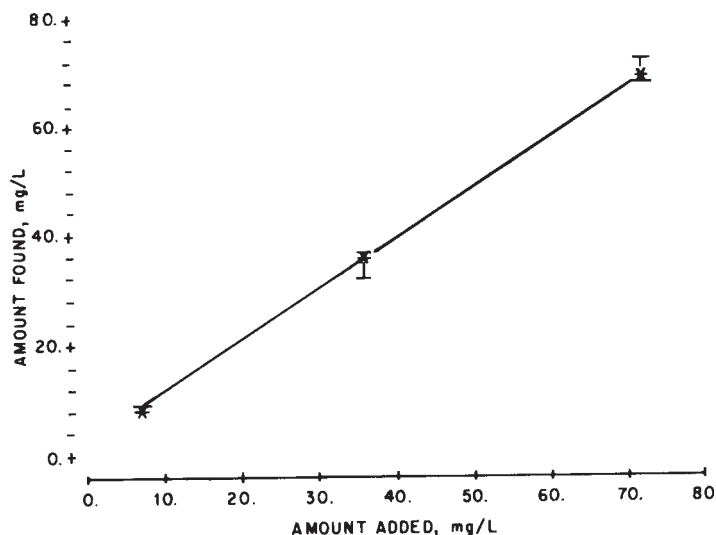


FIG. 4 Plot of Amount Added Versus Amount of Phenol Found in Optional Matrix

TABLE 5 Criteria for Quality Control Requirements

Test Concentration	LCS	Proficiency Demonstration	
	Acceptance Range for LCS	Maximum Acceptable Standard Deviation	Acceptance Range for Mean Recovery
30 µg/L (Method A)	13.0 to 47.0 µg/L	9.51 µg/L	15.3 to 44.7 µg/L
30 mg/L (Method B)	26.6 to 34.4 mg/L	2.00 mg/L	26.1 to 33.9 mg/L

contamination is eliminated and a blank shows no contamination at or above this level, or the results must be qualified with an indication that they do not fall within the performance criteria of the test method.

25.6 Matrix Spike

25.6.1 To check for interferences in the specific matrix being tested, perform an MS on at least one sample from each batch by spiking an aliquot of the sample with a known concentration of C<sub>6</sub>H<sub>5</sub>OH and taking it through the analytical method. Guidance on spiking may be found in Guide D 5810.

25.6.2 The spike concentration plus the background concentration of C<sub>6</sub>H<sub>5</sub>OH must not exceed the concentration of the highest calibration standard used. The spike must produce a concentration in the spiked sample 2 to 5 times the background concentration or 10 to 50 times the detection limit of the test method, whichever is greater.

25.6.3 Calculate the percent recovery of the spike (P) using the following formula:

$$P = \frac{100 [A(V_s + V) - BV_s]}{CV}$$

where:

- $A$  = concentration found in spiked sample,
- $B$  = concentration found in unspiked sample,
- $C$  = concentration of analyte in spiking solution,
- $V_s$  = volume of sample used, and
- $V$  = volume of spiking solution added.

25.6.4 The percent recovery if the spike ( $P$ ) shall fall within the limits calculated following Test Method D 5847, using the collaborative test recession equations for the selected true concentrations used. If the percent recovery is not within these limits, a matrix interference may be present in the sample selected for spiking. Under these circumstances, one of the following remedies must be employed: the matrix interference must be removed, all samples in the batch must be reanalyzed by a test method not affected by the matrix interference, or the results must be qualified with an indication that they do not fall within the performance criteria of the test method.

#### 25.7 Duplicate

25.7.1 To check the precision of sample analyses, analyze a sample in duplicate with each batch. If the concentration of the analyte is less than five times the detection limit for the analyte, an MSD should be used.

25.7.2 Calculate the standard deviation of the duplicate values and compare to the single operator precision in the collaborative study using an  $F$  test. Refer to 6.4.4 of Test Method D 5847 for information on applying the  $F$  test.

25.7.3 If the result exceeds the precision limit, the batch must be reanalyzed or the results must be qualified with an indication that they do not fall within the performance criteria of the test method.

#### 25.8 Independent Reference Material (IRM)

25.8.1 In order to verify the quantitative value produced by the test method, analyze an IRM submitted as a regular sample (if practical) to the laboratory at least once per year. The concentration of the reference material should be in the range appropriate to Method A or B. The value obtained must fall within the control limits specified by the outside source.

## 26. Keywords

256.1 4-aminoantiprene; phenol; phenolic compounds; spectrometry

*ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.*

*This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.*

*This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org).*